


User Guide

Vaisala CARBOCAP® Carbon Dioxide Probe

GMP252

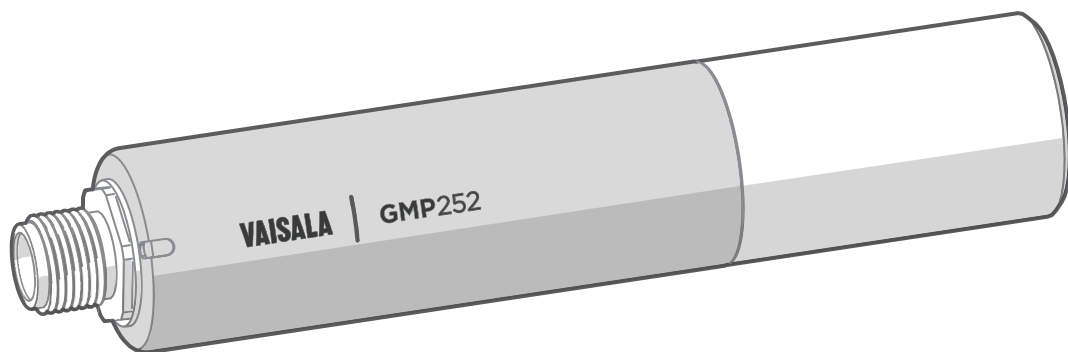

VAISALA

PUBLISHED BY

Vaisala Oyj

Street address: Vanha Nurmijärventie 21, FI-01670 Vantaa, Finland

Mailing address: P.O. Box 26, FI-00421 Helsinki, Finland

Phone: +358 9 8949 1

Visit our Internet pages at www.vaisala.com.

© Vaisala 2018

No part of this manual may be reproduced, published or publicly displayed in any form or by any means, electronic or mechanical (including photocopying), nor may its contents be modified, translated, adapted, sold or disclosed to a third party without prior written permission of the copyright holder. Translated manuals and translated portions of multilingual documents are based on the original English versions. In ambiguous cases, the English versions are applicable, not the translations.

The contents of this manual are subject to change without prior notice.

Local rules and regulations may vary and they shall take precedence over the information contained in this manual. Vaisala makes no representations on this manual's compliance with

the local rules and regulations applicable at any given time, and hereby disclaims any and all responsibilities related thereto.

This manual does not create any legally binding obligations for Vaisala towards customers or end users. All legally binding obligations and agreements are included exclusively in the applicable supply contract or the General Conditions of Sale and General Conditions of Service of Vaisala.

This product contains software developed by Vaisala or third parties. Use of the software is governed by license terms and conditions included in the applicable supply contract or, in the absence of separate license terms and conditions, by the General License Conditions of Vaisala Group.

Table of Contents

1.	About This Document	7
1.1	Version Information	7
1.2	Related Manuals	7
1.3	Documentation Conventions	8
1.4	Trademarks	8
1.5	Patent Notice	9
2.	Product Overview	11
2.1	Introduction to GMP252	11
2.2	Basic Features and Options	12
2.2.1	Connectivity to Vaisala Insight Software	12
2.2.2	Additional Features with Indigo Transmitters	13
2.2.3	Filter Options	13
2.3	Operating Principle of CO ₂ Measurement	14
2.4	Environmental Compensation	15
2.4.1	Temperature Compensation	16
2.4.2	Pressure Compensation	17
2.4.3	Background Gas Compensation	17
2.5	Probe Startup	17
2.6	Filtering Factor	17
2.7	Analog Output Overage Behavior	18
2.7.1	Analog Output Overage Example	18
2.8	Safety	19
2.8.1	ESD Protection	20
2.9	Regulatory Compliances	20
3.	Installation	21
3.1	GMP252 Probe Dimensions	21
3.2	Recommended Installation	21
3.3	Installation Accessories	21
3.3.1	243261SP Mounting Flange	22
3.3.2	243257SP Mounting Clips	23
3.3.3	ASM212017SP Spray Shield	23
3.3.4	DTR250 Radiation Shield	24
3.3.5	DTR250A Pole Mounting Kit	24
3.4	Power Supply	25
3.5	Wiring	25
4.	Vaisala Industrial Protocol	27
4.1	Vaisala Industrial Protocol Overview	27
4.2	Serial Interface Settings	27
4.3	Physical Interface	27
4.4	Connecting with a Computer	27
4.4.1	Installing the Driver for the USB Service Cable	29
4.5	Accessing Serial Commands from Modbus or Analog Mode	30
4.6	Enabling Modbus Mode from Vaisala Industrial Protocol	30
4.7	Changing From Digital Output to Analog Output	31
4.8	Serial Commands	31
4.9	Device Information and Status	33
4.10	Serial Line Output and Communication	36

4.11	Analog Output.....	44
4.12	Calibration and Adjustment.....	49
4.13	Environmental Compensation Commands.....	52
4.14	Other Commands.....	58
5.	Modbus.....	59
6.	Vaisala Insight Software.....	61
6.1	Connecting to Insight Software.....	61
7.	Using GMP252 with Indigo Transmitters.....	63
7.1	Indigo Overview.....	63
7.1.1	Wireless Configuration Interface Overview.....	64
7.2	Taking a Probe in Use with Indigo.....	65
7.2.1	Checking Indigo Support in Probe.....	66
7.3	Attaching Probes and Cables.....	67
7.4	Connecting to Wireless Configuration Interface.....	68
7.5	Logging in to Wireless Configuration Interface.....	69
7.6	Wireless Interface Menus.....	70
7.7	Configuring Analog Outputs with Indigo 201.....	71
7.7.1	Receiving Analog Output Settings from Probe.....	72
7.7.2	Indigo 201 Analog Output Mode Selection.....	72
7.8	Using Modbus with Indigo 202.....	73
7.8.1	Modbus Serial Communication Settings.....	74
7.9	Configuring Relays with Indigo.....	75
7.10	Changing Environmental Compensation Settings with Indigo.....	76
7.11	Configuring Filtering Factor with Indigo.....	77
7.12	Calibrating GMP252 with Indigo.....	78
7.12.1	Indigo Calibration Overview.....	78
7.12.2	Restoring Factory Adjustment.....	80
7.12.3	Calibration PIN Code.....	80
7.12.4	1-point Adjustment with Indigo.....	80
7.12.5	2-point Adjustment with Indigo.....	82
8.	Operating with MI70 Indicator.....	85
8.1	Overview of MI70 Support.....	85
8.1.1	Probe Warm-Up and MI70 Automatic Power Off.....	85
8.2	Basic Display.....	85
8.3	Graphical Display.....	86
8.4	Main Menu.....	86
8.5	Connecting Probe to MI70 Indicator.....	86
8.6	MI70 Indicator Parts.....	87
8.7	Holding and Saving the Display.....	87
8.8	Recording Data.....	88
8.9	Changing Environmental Compensation Settings with MI70 Indicator.....	88
8.10	Calibration and Adjustment with MI70 Indicator.....	89
8.10.1	1-Point Adjustment with an MI70-Compatible Reference Probe.....	90
8.10.2	1-Point Adjustment with a Reference Gas.....	91

9. Maintenance	93
9.1 Cleaning	93
9.1.1 Chemical Tolerance	93
9.2 Changing the Filter	94
9.3 Calibration and Adjustment	94
9.3.1 Calibration Setup	95
9.3.2 Effect of Environmental Compensations	95
9.3.3 Limits of Adjustment	96
9.3.4 Adjustment Types	96
9.3.5 DRW244827SP Calibration Adapter	97
10. Troubleshooting	99
10.1 Problem Situations	99
10.2 Error Messages	99
10.3 Analog Output Error State	100
10.4 Indigo Wireless Connection Troubleshooting	101
11. Technical Data	103
11.1 GMP252 Specifications	103
11.2 Spare Parts and Accessories	106
11.3 GMP252 Probe Dimensions	107
11.4 243261SP Mounting Flange Dimensions	107
11.5 DRW244827SP Calibration Adapter Dimensions	108
11.6 ASM212017SP Spray Shield Dimensions	109
11.7 DTR250 Radiation Shield Dimensions	110
11.8 DTR250A Pole Mounting Kit Dimensions	111
Appendix A: Modbus Reference	113
A.1 Function Codes	113
A.2 Modbus Registers	113
A.2.1 Measurement Data	113
A.2.2 Configuration Registers	114
A.2.3 Status Registers	116
A.2.4 Device Identification Objects	117
A.3 Modbus Communication Examples	118
A.4 Filtering Factor	120
Warranty	121
Technical Support	121
Recycling	121

List of Figures

Figure 1	GMP252 Probe Parts.....	11
Figure 2	ASM212011SP Flow-through Adapter.....	13
Figure 3	Probe Cuvette with Mirror and Sensor Chips.....	14
Figure 4	CO ₂ Measurement in the Measurement Cuvette.....	15
Figure 5	Example of Analog Output Overrange Behavior	19
Figure 6	GMP252 Dimensions.....	21
Figure 7	Probe with 243261SP Mounting Flange.....	22
Figure 8	Probe in 243257SP Mounting Clips.....	23
Figure 9	Probe with ASM212017SP Spray Shield	23
Figure 10	GMP252 in DTR250 Radiation Shield	24
Figure 11	GMP252 Installation with DTR250A Pole Mounting Kit	24
Figure 12	Example of analog output overrange behavior.....	48
Figure 13	Connecting Probe to Insight.....	61
Figure 14	GMP252 Attached to Indigo Transmitter.....	63
Figure 15	Desktop and Mobile Example Views.....	64
Figure 16	Serial Number on Probe Body (GMP251 Example).....	66
Figure 17	Attaching Probes and Cables to Indigo.....	67
Figure 18	Enabling and Accessing Indigo's Wireless Configuration Interface.....	68
Figure 19	Indigo Login View.....	69
Figure 20	Wireless Configuration Interface, Desktop Browser View.....	70
Figure 21	Indigo 201 Analog Output Configuration Options.....	71
Figure 22	Clearing Analog Output Settings	72
Figure 23	Selecting Indigo 201 Analog Output Mode.....	73
Figure 24	Relay Configuration Options.....	75
Figure 25	Calibration Menu Main View.....	78
Figure 26	Start Calibration Button.....	79
Figure 27	MI70 Basic Display.....	85
Figure 28	MI70 Indicator Parts.....	87
Figure 29	CO ₂ Reading with Tcomp and Pcomp on MI70 Screen.....	89
Figure 30	Probe Compensation Settings on MI70 Screen.....	89
Figure 31	Opening the Filter.....	94
Figure 32	DRW244827SP Calibration Adapter with Probe Inserted.....	97
Figure 33	GMP252 Dimensions.....	107
Figure 34	243261SP Mounting Flange Dimensions.....	107
Figure 35	243261SP Mounting Flange Dimensions, Cross Section.....	108
Figure 36	DRW244827SP Calibration Adapter Dimensions.....	108
Figure 37	ASM212017SP Spray Shield Dimensions.....	109
Figure 38	GMP252 Spray Shield Cross Section.....	109
Figure 39	DTR250 Radiation Shield Dimensions (mm).....	110
Figure 40	DTR250A Pole Mounting Kit Dimensions (in mm [inch]).....	111

List of Tables

Table 1	Document Versions.....	7
Table 2	Related Manuals.....	7
Table 3	Applicable Patents.....	9
Table 4	Analog Output Overrange Clipping and Error Limits.....	18
Table 5	M12 Male Connector.....	25
Table 6	Default Serial Interface Settings.....	27
Table 7	Basic Serial Commands.....	32
Table 8	Advanced Serial Commands.....	33
Table 9	? Command.....	33
Table 10	Errs Command.....	34
Table 11	Help Command.....	34
Table 12	Snum command.....	35
Table 13	System Command.....	35
Table 14	Time Command.....	36
Table 15	Vers Command.....	36
Table 16	Addr Command.....	36
Table 17	Close Command.....	37
Table 18	Form Command.....	37
Table 19	Output Parameters for Form Command.....	39
Table 20	Modifiers for Form Command.....	39
Table 21	Intv Command.....	40
Table 22	Open Command.....	40
Table 23	R Command.....	41
Table 24	S Command.....	41
Table 25	Sdelay Command.....	42
Table 26	Send Command.....	42
Table 27	Seri Command.....	42
Table 28	Smode Command.....	43
Table 29	Amode Command.....	44
Table 30	Aover Command.....	45
Table 31	Asel Command.....	48
Table 32	Adate Command.....	49
Table 33	Atext Command.....	49
Table 34	Cdate Command.....	50
Table 35	Ctext Command.....	50
Table 36	CCO2 Command.....	50
Table 37	Env Command.....	53
Table 38	O2cmode Command.....	55
Table 39	Pcmode Command.....	56
Table 40	Rhcmode Command.....	56
Table 41	Tcmode Command.....	57
Table 42	Frestore Command.....	58
Table 43	Pass Command.....	58
Table 44	Reset Command.....	58
Table 45	Default Modbus Serial Communication Settings.....	59
Table 46	Indigo 202 Modbus Registers.....	73
Table 47	Measurement Performance.....	103
Table 48	Operating Environment.....	104
Table 49	Mechanical Specifications.....	104
Table 50	Inputs and Outputs.....	105
Table 51	Supported Function Codes.....	113

Table 52 Modbus Measurement Data Registers (Read-Only).....113

Table 53 Modbus Configuration Data Registers (Writable)..... 114

Table 54 Modbus Status Registers (Read-Only)..... 116

Table 55 Device Identification Objects.....117

1. About This Document

1.1 Version Information

Table 1 Document Versions

Document Code	Date	Description
M211897EN-D	March 2018	<ul style="list-style-type: none"> Added information about using the probe with Vaisala Insight PC software. PuTTY terminal settings instructions updated. Calibration uncertainty specification updated. DTR250A radiation shield pole mounting kit added. Added recommendation to disable MI70 indicator's automatic power off feature when used with GMP252. Updated instructions on using MI70 to configure environmental compensations. Default device address in serial line communication corrected (240). Corrected the unit information of sdelay command. Added a note about maximum voltage output to analog error state output configuration. Information on Modbus register numbers updated.
M211897EN-C	June 2017	<ul style="list-style-type: none"> Added information about using the probe with Vaisala Indigo transmitters. Added flow-through adapter accessory ASM212011SP, spray shield accessory ASM212017SP, and radiation shield accessory DTR250. Modbus status register information updated. Calibration adapter order code corrected.
M211897EN-B	August 2016	Modbus status register values and descriptions updated.

1.2 Related Manuals

Table 2 Related Manuals

Document Code	Description
M211893EN	Vaisala CARBOCAP® Carbon Dioxide Probe GMP252 Quick Guide
M211799EN	Vaisala CARBOCAP® Carbon Dioxide Probe GMP251 User Guide
M211798EN	Vaisala CARBOCAP® Carbon Dioxide Probe GMP251 Quick Guide
M211877EN	Vaisala Indigo™ 201 Analog Output Transmitter User Guide

Document Code	Description
M211876EN	Vaisala Indigo™ 201 Analog Output Transmitter Quick Guide
M211966EN	Vaisala Indigo™ 202 Digital Transmitter User Guide
M211967EN	Vaisala Indigo™ 201 Digital Transmitter Quick Guide

1.3 Documentation Conventions



WARNING! alerts you to a serious hazard. If you do not read and follow instructions carefully at this point, there is a risk of injury or even death.



CAUTION! warns you of a potential hazard. If you do not read and follow instructions carefully at this point, the product could be damaged or important data could be lost.



Note highlights important information on using the product.



Tip gives information for using the product more efficiently.

1.4 Trademarks

Vaisala® and CARBOCAP® are registered trademarks of Vaisala Oyj.

Windows® is either a registered trademark or trademark of Microsoft Corporation in the United States and other countries.

All other product or company names that may be mentioned in this publication are trade names, trademarks, or registered trademarks of their respective owners.

1.5 Patent Notice

This product is protected by the following patents and their corresponding national rights:

Table 3 [Applicable Patents](#)

Patent Issued By	Patent Number
United States Patent and Trademark Office	US 5,827,438
	US 6,177,673
European Patent Office	EP0776023
	EP0922972
German Patent and Trade Mark Office	69615635
Japan Patent Office	4263285
Finnish Patent Office	112005
	105598

2. Product Overview

2.1 Introduction to GMP252

GMP252 is designed for CO₂ measurement in demanding applications that require reliable and accurate performance. The measurement range is 0 ... 10 000 ppmCO₂ (measurements can be carried out in the 10 000 ... 30 000 ppmCO₂ range with reduced accuracy).

The probe is based on Vaisala's patented 2nd generation CARBOCAP® technology and equipped with Vaisala's Microglow infrared light source. The probe is easy to install with a plug-in/plug-out M12 connection.

GMP252 is able to compensate for temperature, pressure and background gas. For temperature compensation purposes, the probe includes an internal temperature sensor that allows measurement compensation according to ambient temperature. As dust and most chemicals do not affect the measurement, and the effect of temperature, pressure and background gas can be compensated for, GMP252 can provide accurate and stable measurements in a wide range of applications.

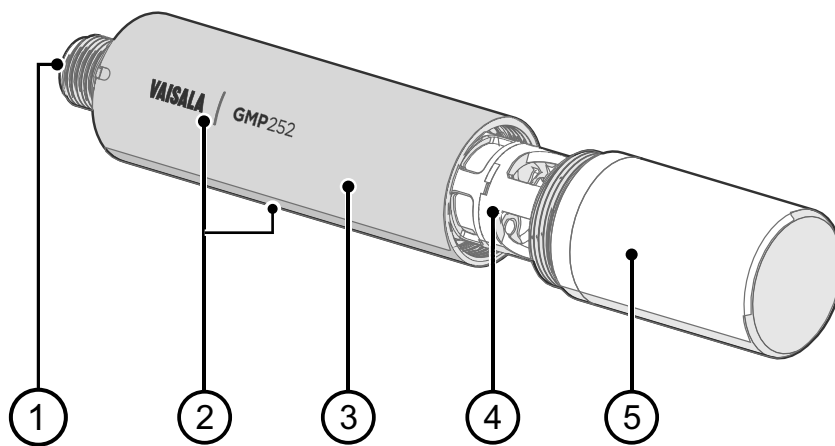


Figure 1 GMP252 Probe Parts

- 1 5-pin M12 connector. For pinout, see [Wiring \(page 25\)](#).
- 2 Probe name and orientation mark for Vaisala transmitter installations (front) and laser-printed type label (back).
- 3 Probe body. Contains the main component board.
- 4 Measurement cuvette with optics and CARBOCAP® CO₂ sensor.
- 5 Filter (sintered, PTFE: see also [Filter Options \(page 13\)](#)).



CAUTION! Do not attempt to open the probe body. There are no user serviceable parts inside the probe body.

2.2 Basic Features and Options

- CO₂ measurement range 0 ... 10 000 ppmCO₂.
- Measurement up to 30 000 ppmCO₂ with reduced accuracy.
- Operating temperature range -40 ... +60 °C (-40 ... +140 °F).
- Vaisala CARBOCAP® CO₂ sensor with excellent long-term stability.
- Measurement compensated for effects of temperature, pressure, and background gas. The temperature compensation can be based on an integrated temperature sensor or use a set temperature. Pressure and background gas parameters can be set to the probe.
- Heating to avoid condensation on optical elements.
- Digital output with RS-485:
 - Modbus RTU
 - Vaisala Industrial Protocol
- Analog output:
 - Current output (0 ... 20 mA or 4 ... 20 mA)
 - Voltage output (0 ... 5 V or 0 ... 10 V)
- Can be used as a stand-alone probe or with Vaisala Indigo transmitters.
- Can be connected to Vaisala Insight software for configuration, diagnostics, and temporary online monitoring.
- Compatible with MI70 hand-held meter.
- Easy plug-in, plug-out.

More Information

- [GMP252 Specifications \(page 103\)](#)
- [Operating Principle of CO₂ Measurement \(page 14\)](#)
- [Environmental Compensation \(page 15\)](#)
- [Vaisala Industrial Protocol Overview \(page 27\)](#)
- [Modbus \(page 59\)](#)
- [Overview of MI70 Support \(page 85\)](#)

2.2.1 Connectivity to Vaisala Insight Software

The probe can be connected to Vaisala Insight software using a Vaisala USB cable (no. 242659). With the Insight software, you can:

- Calibrate and adjust the measurement.
- See device information and status.
- See real-time measurement.
- Configure serial communication settings, purge settings, filtering factor, and analog output parameters and scaling.

More Information

- [Connecting to Insight Software \(page 61\)](#)

2.2.2 Additional Features with Indigo Transmitters

GMP252 probes manufactured from 2017 onwards are compatible with Vaisala Indigo transmitters. Connecting the probe to an Indigo transmitter provides a range of additional options for outputs, measurement viewing, status monitoring, and configuration interface access.

Examples of additional features available with Indigo transmitters include:

- 3.5" TFT LCD color display or non-display model with LED indicator
- Digital output or 3 analog outputs (depending on the transmitter model)
- 2 configurable relays
- Wireless browser-based configuration interface for mobile devices and computers (IEEE 802.11 b/g/n WLAN)

The selection of available additional features (for example, output and connectivity options) varies depending on the Indigo transmitter model. For more information on Indigo transmitters, see www.vaisala.com/indigo.

More Information

- [Indigo Overview \(page 63\)](#)

2.2.3 Filter Options


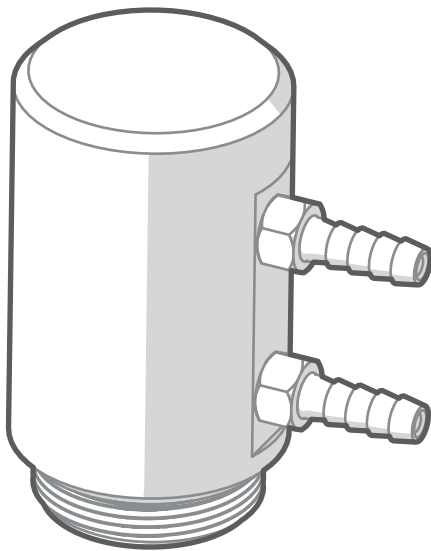


Figure 2 ASM212011SP Flow-through Adapter

The GMP252 flow-through adapter (order code ASM212011SP) has two gas ports for controlled gas feed (port outer diameter 4.6 mm, port hole inner diameter 2 mm, suitable for tubing with 4 mm inner diameter). For information on ordering accessories and spare parts, see [Spare Parts and Accessories \(page 106\)](#).

2.3 Operating Principle of CO₂ Measurement

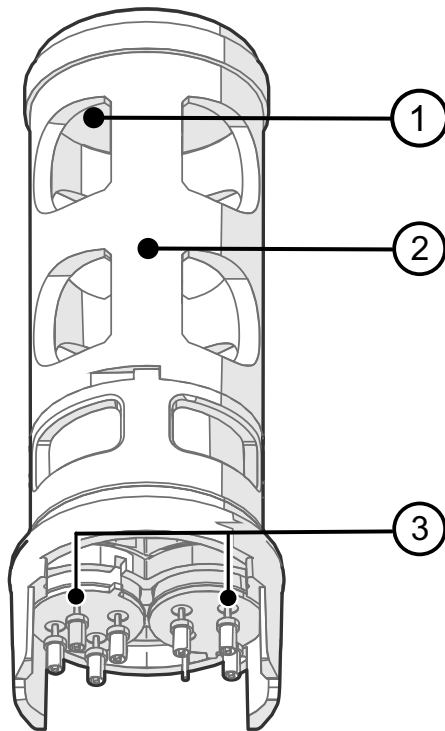

The Vaisala CARBOCAP® sensor used in the probe is a silicon-based, nondispersive infrared (NDIR) sensor for measurement of gaseous carbon dioxide in air-like gases.

Figure 3 Probe Cuvette with Mirror and Sensor Chips

- 1 Mirror
- 2 Cuvette
- 3 Sensor chips under TO5 package

The sensitivity to carbon dioxide is based on absorption of infrared light at a characteristic wavelength. During measurement, infrared light is routed through the cuvette that contains the gas to be measured. A mirror reflects the light from the cuvette to a thermopile detector that measures the light intensity at a wavelength determined by a Fabry-Pérot interferometer (FPI) and a band pass filter.

The carbon dioxide measurement consists of two steps: first, the FPI is electrically tuned so that its pass band coincides with the characteristic absorption wavelength of carbon dioxide and the signal is recorded. Second, the pass band is shifted to a wavelength where no absorption occurs in order to get a reference signal. The ratio of these two signals, one at the absorption wavelength and the other at the reference wavelength, gives the fraction of light absorption from which the carbon dioxide concentration is calculated. Measuring the reference signal compensates the possible effects of sensor aging and signal attenuation due to dirt on optical surfaces, making the sensor very stable over time.

TO5 packages with hermetic windows are used to protect the sensor chips from moisture and contamination. A heater chip is utilized to prevent condensation in normal operation.

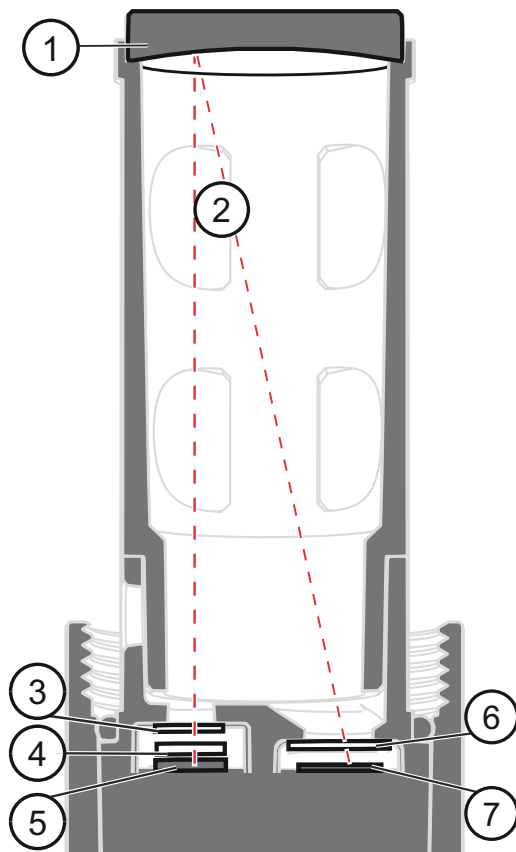


Figure 4 CO₂ Measurement in the Measurement Cuvette

- 1 Gold-plated mirror
- 2 Light absorbed by CO₂ in the measured gas
- 3 Hermetic window
- 4 Fabry-Pérot interferometer
- 5 Light source (Microglow)
- 6 Hermetic window
- 7 Thermopile detector

2.4 Environmental Compensation

When necessary, various environmental compensations can be applied to improve the CO₂ measurement accuracy of the probe.

The probe can compensate for the effects of the following parameters:

- Temperature
- Pressure
- Background gas oxygen (O₂) content
- Background gas relative humidity (%RH)



To apply an accurate relative humidity compensation, make sure that also the temperature compensation and pressure compensation configurations match the measurement environment.

The probe has an on-board temperature sensor that can be used to compensate for temperature. Additionally, if the probe is integrated in a system that measures one or more of the compensation parameters (T, P, RH, O₂), they can be updated to the probe continuously.

Compensation parameters are configured on the order form when ordering the probe, and can later be updated using Vaisala Industrial Protocol or Modbus protocol.

You can also turn off any of the compensations. In that case, the probe uses the default compensation value that is mathematically neutral for the probe's internal compensation model.

You can configure the environmental compensation settings with any of the following options:

- Vaisala Industrial Protocol serial commands
- Vaisala Insight software
- Indigo transmitter's wireless configuration interface
- Modbus configuration registers
- MI70 hand-held indicator



The environmental compensation configuration options available in the MI70 handheld indicator are not compatible with the probe. Using MI70 to configure the environmental compensation settings of the probe can decrease measurement accuracy.

More Information

- [Effect of Environmental Compensations \(page 95\)](#)
- [Environmental Compensation Commands \(page 52\)](#)
- [Vaisala Insight Software \(page 61\)](#)
- [Changing Environmental Compensation Settings with Indigo \(page 76\)](#)
- [Configuration Registers \(page 114\)](#)
- [Changing Environmental Compensation Settings with MI70 Indicator \(page 88\)](#)

2.4.1 Temperature Compensation

The probe can measure the approximate temperature of the CARBOCAP® sensor for compensation, or use a fixed setpoint. Unless a dedicated temperature measurement is available and can be regularly updated to the probe, it is strongly recommended to use the probe's internal temperature compensation to ensure real-time accurate measurements. If the measurement is made in a constant temperature, the constant temperature can be set as the compensation value (fixed setpoint option).

If temperature compensation is turned off, the probe uses the default value of +25 °C (+77 °F).



When the probe is installed through a flange and part of the probe and the cable is left outside the measuring environment, it is possible that temperature conduction from the probe body and cable outside the measurement environment affects the temperature compensation and decreases measurement accuracy.

2.4.2 Pressure Compensation

The probe does not have on-board pressure measurement. However, a pressure reading from an external source can be used as a setpoint value for compensation using Vaisala Industrial Protocol or Modbus.

If pressure compensation is turned off, the probe uses the default compensation value of 1013 hPa.

2.4.3 Background Gas Compensation

The probe does not have on-board oxygen or relative humidity measurement. However, oxygen and relative humidity readings from an external source can be used as setpoint values for compensation using Vaisala Industrial Protocol or Modbus. The default setpoint values are as follows:

- Oxygen concentration: 0 %O₂ or 21 %O₂
- Relative humidity: 0 %RH or 50 %RH

If background gas compensations are turned off, the probe uses the value 0 % for both.

In practice, when CO₂ is measured at a ppm level, O₂ and RH compensations have a very small effect on the accuracy of the measurement.

2.5 Probe Startup

When powered on, the probe starts up within 12 seconds. Measurements from the outputs (digital and analog) become available during this time but note that they will only reach specified accuracy after a 2-minute warm-up period. For this reason, you should design your system so that it does not rely on measurements from the probe during this time. When the probe is in analog output mode, the probe remains in an error state during the start-up phase until measurement output becomes available.



Specifically note that the CO₂ reading will rise to the correct reading as the sensor's infrared emitter achieves operating temperature.

2.6 Filtering Factor

You can set a filtering factor that affects the speed at which the latest CO₂ measurement is integrated into the output of the probe. This allows averaging the output if the measuring environment produces occasional exceptionally high or low readings.

The filtering factor can be set either with Modbus configuration registers or with an Indigo transmitter's wireless configuration interface.

More Information

- [Configuration Registers \(page 114\)](#)
- [Configuring Filtering Factor with Indigo \(page 77\)](#)

2.7 Analog Output Overrange Behavior

The analog output of the probe has a defined behavior when the values measured by the probe are outside the scaled analog output range. At first, the output is clipped when the measurement exceeds a set limit (the measurement continues, but the output does not change from the clipped value).

When the measurement exceeds the second limit (error limit), the analog output switches to the error state defined for the output.

The table below lists the clipping and error limits and default error state outputs for the analog voltage and current outputs.

Table 4 Analog Output Overrange Clipping and Error Limits

Output Voltage / Current	Clipping Limit	Error Limit	Default Error State Output
0 ... 5 V	>5 %	>10 %	0 V
0 ... 10 V	>1 %	>10 %	0 V
0 ... 20 mA	>5 %	>10 %	23 mA
4 ... 20 mA	>5 %	>10 %	2 mA

The same clipping and error limits are applied when the measured value drops back to the scaled range: at first the output returns to the clipped value from the error state, and then to normal output.



Clipping and error state limits differ for 0 ... 10 V and 0 ... 5 V outputs. For 0 ... 10 V output the limits are 1 % and 10 %, and for 0 ... 5 V output the limits are 5 % and 10 %.



When setting the error output voltage (**amode** command), note that the probe's maximum voltage output is 10.325 V.

More Information

- [Analog Output Error State \(page 100\)](#)
- [Analog Output \(page 44\)](#)

2.7.1 Analog Output Overrange Example

Consider a probe with 0 ... 5 V output, scaled to 0 ... 2000 ppmCO₂.

- When the measured CO₂ rises above 2000 ppmCO₂, the output rises above 5 V.
- The output keeps rising until the measurement is 2100 ppmCO₂, at which point the probe outputs 5.25 V.
- If the CO₂ level rises above 2100 ppmCO₂, the output still remains at 5.25 V.
- If the CO₂ level rises above 2200 ppmCO₂, the output enters the error state, which is 0 V for the 0 ... 5 V output.

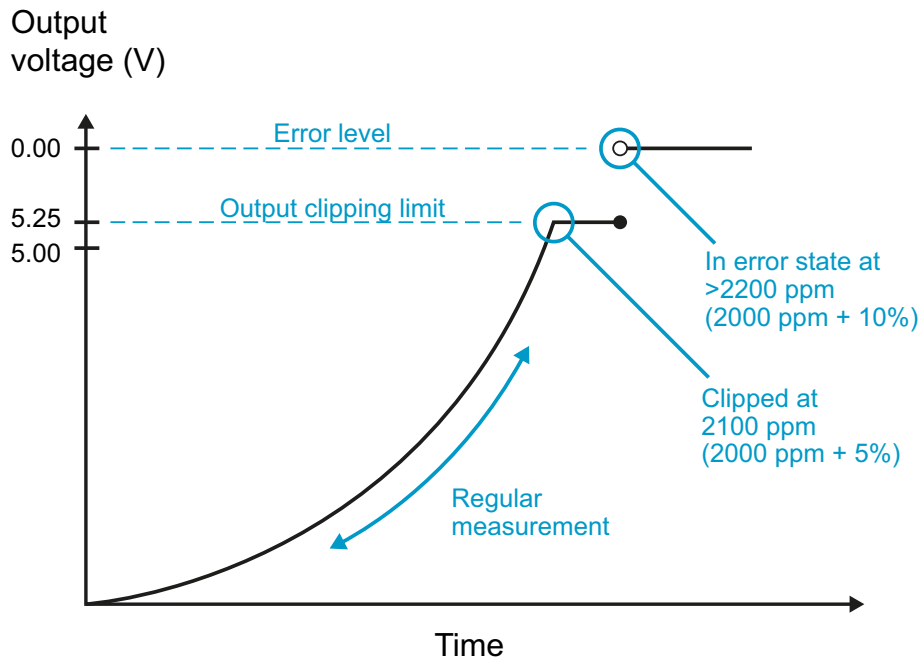


Figure 5 Example of Analog Output Overrange Behavior

This example uses output scaled to 0 ... 5 V and 0 ... 2000 ppmCO₂, error level set to 0 V, clipping set to 5 % overrange, and error limit set to 10 % overrange. CO₂ concentrations (ppm) are indicated for the clipping point and error limit point.



This overrange and error behavior is specific to the analog output, and does not affect the readings of the digital outputs.

You can change the analog output overrange behavior using the **aover** command.

2.8 Safety

The probe delivered to you has been tested for safety and approved as shipped from the factory. Note the following precautions:



WARNING! When returning a product for calibration or repair, make sure it has not been exposed to dangerous contamination, and is safe to handle without special precautions.



CAUTION! Do not modify the unit or use it in ways not described in the documentation. Improper modification may lead to safety hazards, equipment damage, failure to perform according to specification, or decreased equipment lifetime.



CAUTION! Do not attempt to open the probe body. There are no user serviceable parts inside the probe body.

2.8.1 ESD Protection

Electrostatic Discharge (ESD) can cause immediate or latent damage to electronic circuits. Vaisala products are adequately protected against ESD for their intended use. However, it is possible to damage the product by delivering electrostatic discharges when touching an exposed contact on the product.

To make sure you are not delivering high static voltages yourself, avoid touching the pins on the M12 connector.

2.9 Regulatory Compliances

The probe is in conformity with the provisions of the following EU directives:

- RoHS Directive
- EMC Directive

Conformity is shown by compliance with the following standards:

- EN 50581: Technical documentation for the assessment of electrical and electronic products with respect to the restriction of hazardous substances.
- EN 61326-1: Electrical equipment for measurement, control, and laboratory use – EMC requirements – Generic environment.
- EN 55022: Information technology equipment – Radio disturbance characteristics – Limits and methods of measurement.

3. Installation

3.1 GMP252 Probe Dimensions

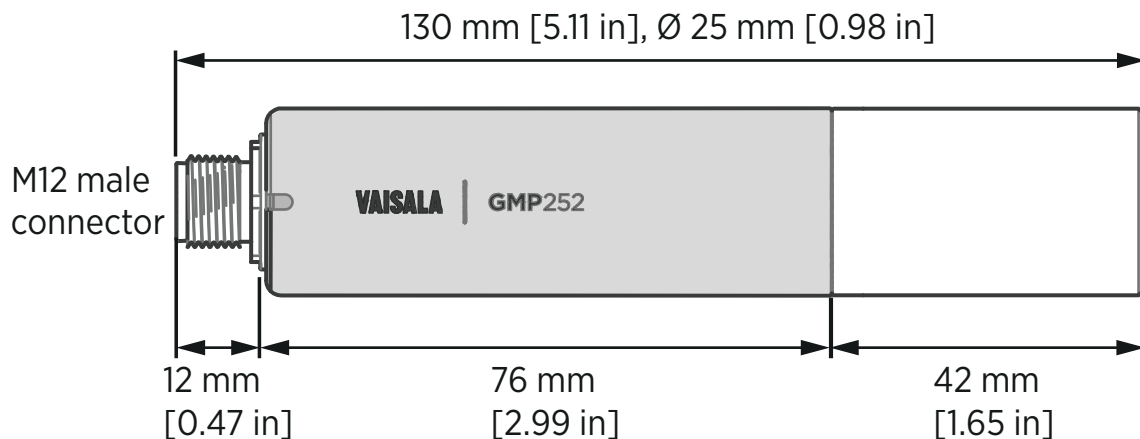


Figure 6 GMP252 Dimensions

3.2 Recommended Installation

The probe can be installed in an environment with an operating temperature range -40 ... +60 °C (-40 ... +140 °F). Make sure the probe is in a location that represents the measurement environment properly.

The 5-pin male M12 connector on the probe provides an easy plug-in/plug-out connection to a compatible cable.

3.3 Installation Accessories

The probe can be installed through a surface using the optional flange accessory (Vaisala product code 243261SP), or attached for example to a wall with the optional clip accessory (two-clip set, Vaisala product code 243257SP).

For installations where a pressure washer is used to clean the measurement area, a spray shield with an IP9X rating (Vaisala product code ASM212017SP) is available as an optional accessory.

If the probe is installed outdoors, the optional DTR250 radiation shield accessory can be used to protect the probe from solar radiation and precipitation. The radiation shield can be ordered either as a stand-alone item with an integrated mounting plate, or together with a pole mounting kit.

More Information

- [Spare Parts and Accessories \(page 106\)](#)

3.3.1 243261SP Mounting Flange

The optional flange accessory is used to install the probe body through a wall or other surface.

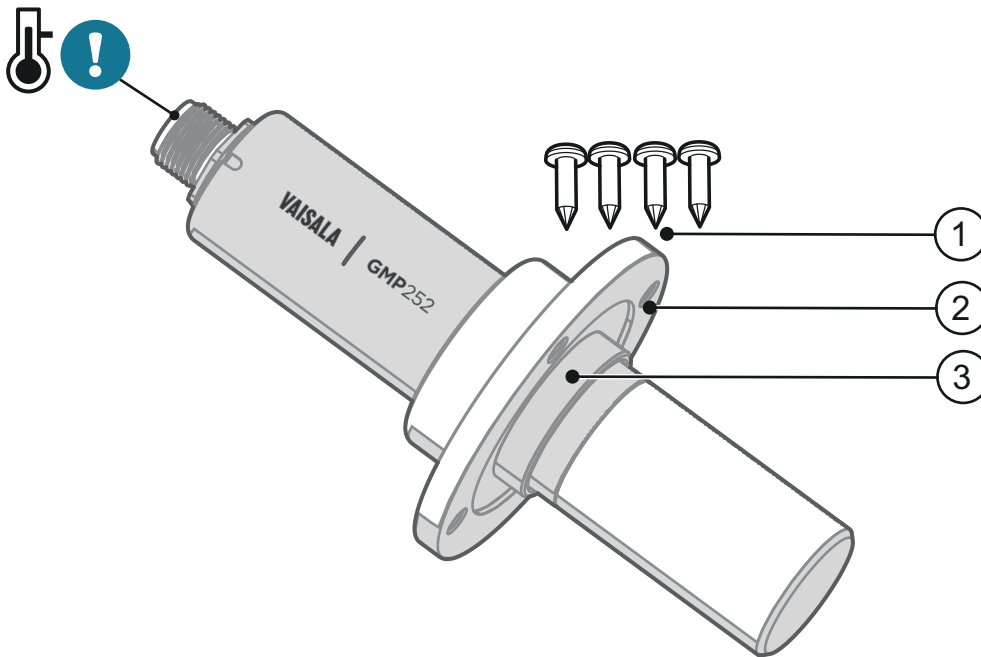


Figure 7 Probe with 243261SP Mounting Flange

- 1 4 Phillips head screws (included)
- 2 Mounting flange (diameter 60 mm) with four Ø 4.2 mm screw holes
- 3 Gasket ring



Leaving part of the probe body and the cable outside the measurement environment can cause heat conduction that affects the temperature compensation and measurement accuracy.

More Information

- [243261SP Mounting Flange Dimensions \(page 107\)](#)

3.3.2 243257SP Mounting Clips

The optional mounting clips (set of two clips) are used to hold the probe in place for example on a wall or other surface. Each clip base attaches to the installation surface with one screw (screw hole Ø 4.2 mm).

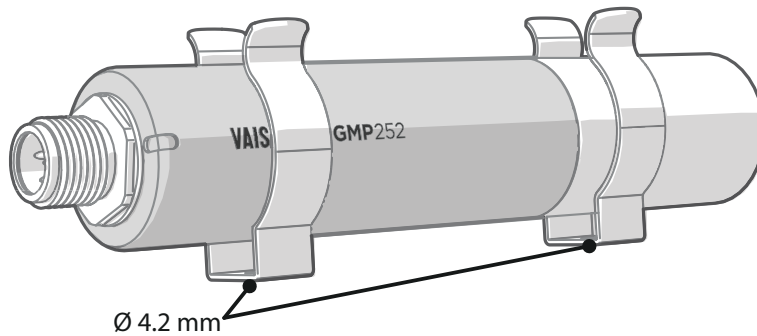


Figure 8 Probe in 243257SP Mounting Clips

3.3.3 ASM212017SP Spray Shield

The optional spray shield (Vaisala order code: ASM212017SP) allows washing the probe with a pressure washer without exposing the sensor to moisture (IP9X rating).

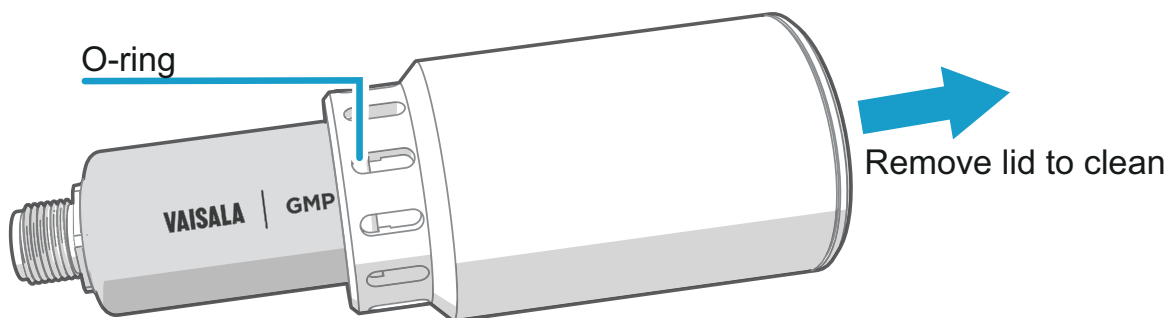


Figure 9 Probe with ASM212017SP Spray Shield



The spray shield can limit or prevent the use of the probe mounting clips (243257SP).

More Information

- [ASM212017SP Spray Shield Dimensions \(page 109\)](#)

3.3.4 DTR250 Radiation Shield

The optional DTR250 radiation shield (Vaisala order code: DTR250) protects the probe from solar radiation and precipitation in outdoor installations.

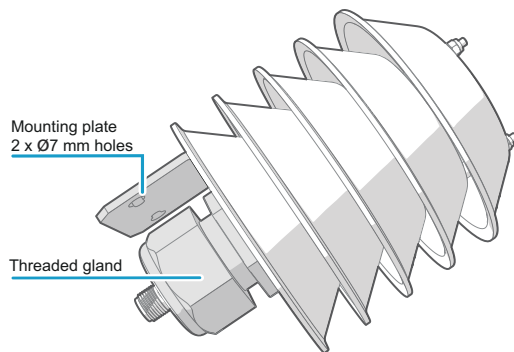


Figure 10 GMP252 in DTR250 Radiation Shield

More Information

- [DTR250 Radiation Shield Dimensions \(page 110\)](#)

3.3.5 DTR250A Pole Mounting Kit

The DTR250A pole mounting kit (Vaisala order code: DTR250A) includes the DTR250 radiation shield and an installation kit for pole masts (pole mast diameter: 30 ... 60 mm).

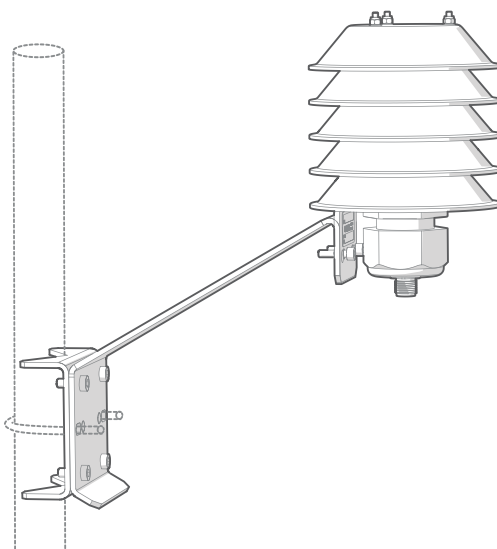


Figure 11 GMP252 Installation with DTR250A Pole Mounting Kit

More Information

- [DTR250A Pole Mounting Kit Dimensions \(page 111\)](#)

3.4 Power Supply

The supply voltage range of the probe is 12 ... 30 VDC with the digital output option. If the analog output is used, the supply voltage range is 12 ... 30 VDC for voltage output and 20 ... 30 VDC for current output.

Typical power consumption is less than 0.4 W in continuous operation, and the maximum is 0.5 W.

More Information

▸ [GMP252 Specifications \(page 103\)](#)

3.5 Wiring




Table 5 M12 Male Connector

Pin#	Function	Note	Cable 223263SP Wire Colors
1	Power in	<ul style="list-style-type: none"> • With digital output: 12 ... 30 VDC • With voltage output: 12 ... 30 VDC • With current output: 20 ... 30 VDC Typical average power consumption <0.4 W, maximum 0.5 W.	Brown
2	RS-485- or voltage output	Voltage: 0 ... 5 VDC or 0 ... 10 VDC (default analog output scaling)	White
3	GND	–	Blue
4	RS-485 + or current output	Current: 0 ... 20 mA or 4 ... 20 mA (default analog output scaling)	Black
5	Output control	Connecting pin #5 to GND (pin #3) forces the probe to analog output mode. If an analog output configuration has not been selected, default 0 ... 10 VDC and 4 ... 20 mA scalings are used. If pin #5 is not connected, the analog or digital output selected when ordering or set later through configuration is used.	Gray



Note that the probe always remains in analog mode when pin #5 is connected to pin #3, and cannot be switched to digital output in this wiring option.

4. Vaisala Industrial Protocol

4.1 Vaisala Industrial Protocol Overview

The RS-485 line of the probe provides an implementation of the Vaisala Industrial Protocol that can be used for service and configuration use, or for interfacing with the system to which the probe is integrated. The protocol is a plaintext protocol suitable for use both by human operators and automated systems.

4.2 Serial Interface Settings

Table 6 Default Serial Interface Settings

Property	Description/Value
Bit rate	19200
Parity	None
Data bits	8
Stop bit	1
Flow control	None

4.3 Physical Interface

The physical interface is a non-isolated 2-wire interface. The data lines are RS-485 D- and RS-485 D+. Ground is shared with power supply. The connector is a 5-pin male M12.

More Information

- [Wiring \(page 25\)](#)


4.4 Connecting with a Computer



- Vaisala USB service cable (order code 242659)
- Computer with:
 - Windows operating system
 - Terminal application (for example PuTTY, available from www.vaisala.com/software)
 - Free USB port
 - Driver for Vaisala USB service cable installed (available on the cable installation media and at www.vaisala.com/software)

The steps below describe how to connect to the probe using the PuTTY terminal application for Windows and a USB computer connection cable. Connecting with a computer allows you to configure and troubleshoot your probe using serial line commands.

- ▶ 1. If you have not used the Vaisala USB cable before, install the driver before attempting to use the cable.
2. Connect the USB serial interface cable between your computer and the M12 connector of the probe.
3. Start the PuTTY application.
4. Select **Connection > Serial & USB** and check that the correct COM port is selected in the **Serial or USB line to connect to** field. If you are using the PuTTY terminal application supplied by Vaisala, you can press the **USB Finder** button to open the Vaisala USB Instrument Finder program.
5. Check that the other serial settings are correct for your connection, and change if necessary. **Flow control** should be set to **None** unless you have a reason to change it.

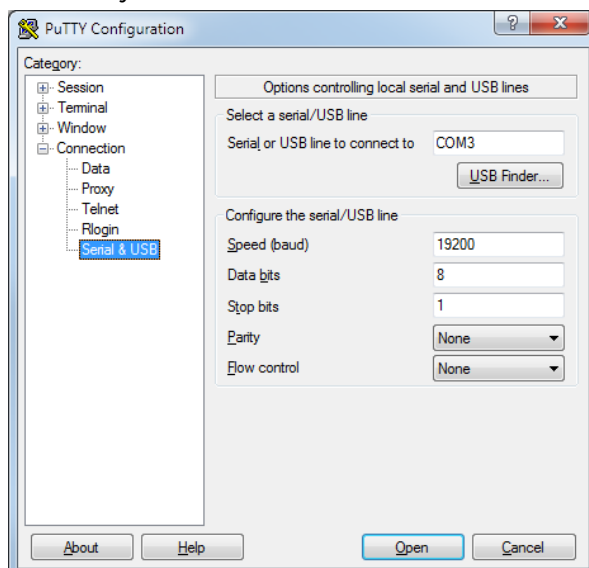

6. Select **Terminal**. Use the following settings:
Local Echo: Select **Force on**. This setting ensures that your typing is shown on the session window.



CAUTION! Make sure that the **Send line ends with line feeds (CR+LF)** option is not selected. Enabling this option can cause issues with the terminal connection.

7. To open the connection window and start using the serial line, select **Open**.



If PuTTY is unable to open the serial port you selected, it shows you an error message instead. If this happens, restart PuTTY and check the settings.

More Information


- [Serial Interface Settings \(page 27\)](#)
- [Installing the Driver for the USB Service Cable \(page 29\)](#)

4.4.1 Installing the Driver for the USB Service Cable



Only Windows® operating systems are supported by the driver of the USB service cable.

- ▶ 1. Connect the USB service cable to a USB port on your computer. Windows® detects the new device and installs the appropriate driver.
2. Open **Devices and Printers** from the Windows® Start menu. Use search to find it if necessary (search for "devices").
3. Locate the cable in the list of devices:
 - If the device is listed as **Vaisala USB Device** with a COM port number in brackets, the cable is ready for use. **Note the COM port number, you will need it later.**
 - If the device is listed as **Vaisala USB Instrument Cable** without a COM port number listed, you must install the driver manually.

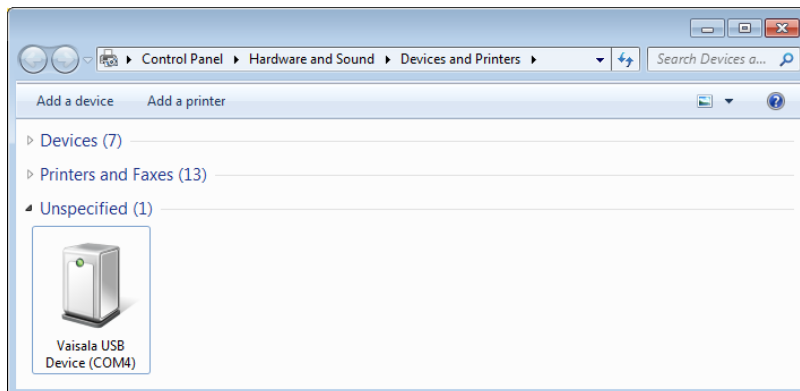

4. To install the driver manually:
 - a. Disconnect the USB service cable from the computer.
 - b. Download the Vaisala USB driver at <http://www.vaisala.com/software> (select the appropriate USB Instrument Driver Setup for your cable).
 - c. Run the USB driver installation program *Vaisala USB Device Driver Setup.exe*. Accept the installation defaults.
 - d. Go back to [step 1](#) and verify that the driver installation works as expected.

4.5 Accessing Serial Commands from Modbus or Analog Mode

- ▶ 1. Connect the USB cable to your PC and start the terminal application as instructed in [Connecting with a Computer \(page 27\)](#).
2. Start a new terminal session using the default serial settings.
3. Keep the Enter key pressed down and connect the probe to the USB cable. When the probe is powered on (connected to your PC with the USB cable), you must send five carriage returns (Enter key presses) within 0.7 seconds to force the probe to serial command mode. The probe model information appears in the terminal application when the mode has been successfully changed, and Vaisala Industrial Protocol commands are available for use.
4. To test the connection, enter for example the **?** command. If the mode change failed, close the terminal application, disconnect the probe from the USB cable, and repeat [step 2](#) and [step 3](#).
5. To keep the serial mode in use (forced serial mode access is temporary and switches off at reset), select a serial output option (stop/run/poll) with the **smode** command.



Note that the probe always remains in analog mode when pin #5 is connected to pin #3, and cannot be switched to digital output in this wiring option.

More Information

- ▶ [Serial Interface Settings \(page 27\)](#)
- ▶ [Enabling Modbus Mode from Vaisala Industrial Protocol \(page 30\)](#)

4.6 Enabling Modbus Mode from Vaisala Industrial Protocol

If you need to switch from Vaisala Industrial Protocol to Modbus mode, you must configure the following settings:

- Serial line operating mode
 - Modbus address
 - Serial line settings (bit rate, parity, stop and data bits)
- ▶ 1. Connect the USB cable to your PC and start the terminal application as instructed in [Connecting with a Computer \(page 27\)](#).

2. Set the serial mode to Modbus with the **smode** command:

```
smode modbus
```

3. Set the Modbus address to 240 with the **addr** command:

```
addr 240
```

4. Set the serial line settings to 19200/N/8/2 with the **seri** command:

```
seri 19200 N 8 2
```

5. Power off (disconnect) the probe or reset with the **reset** command. The new configuration is available at the next restart.

More Information

- [Accessing Serial Commands from Modbus or Analog Mode \(page 30\)](#)

4.7 Changing From Digital Output to Analog Output

- ▶ 1. Set up a terminal connection as instructed in [Connecting with a Computer \(page 27\)](#).
- 2. Change the mode from digital to analog with the **smode** serial command: **smode analog**.
- 3. Reset the probe (disconnect and reconnect the cable or use the **reset** serial command) to power on in analog output mode.

More Information

- [Accessing Serial Commands from Modbus or Analog Mode \(page 30\)](#)

4.8 Serial Commands

The notation **<cr>** refers to the carriage return control character, which you can send in a terminal application by pressing enter on your keyboard. Before entering commands, send a **<cr>** to clear the command buffer.

You can enter the commands in uppercase or lowercase. In the command examples, the keyboard input by the user is in bold type.

Table 7 (page 32) lists the basic serial commands that are available by default. To access advanced serial commands (listed in Table 8 (page 33)), enter the command **pass 1300**.

Table 7 Basic Serial Commands

Command	Description
Device information and status	
?	Show probe information.
??	Show probe information (will respond in POLL mode).
errs	Show currently active errors.
help	Show list of currently available serial commands.
snum	Show probe serial number.
system	Show probe firmware information.
time	Show probe operation hours and uptime.
vers	Show probe firmware version.
Serial line output and communication	
close	Close connection to probe (POLL mode)
form [modifier string]	Show or set output format.
intv [0 ... 255 s/min/h]	Set continuous output interval for R command.
open [address]	Open connection to probe in POLL mode.
r	Start the continuous outputting.
s	Stop the continuous outputting.
sdelay [1 ... 255]	Show or set serial line transmission delay (1 ... 255, 1 unit = 4 milliseconds)
send	Output a single measurement message.
seri [baud data stop parity]	Show or set the serial interface settings.
smode [mode]	Show or set startup serial mode: RUN , STOP , or POLL .
Environmental compensation	
env	Show or set environmental parameters.
Adjustment information	
adate	Show CO ₂ factory adjustment date.
atext	Show CO ₂ factory adjustment information.
Other commands	
reset	Reset the probe.
pass [1300]	Access advanced serial commands.

Table 8 Advanced Serial Commands

Command	Description
Serial line output and communication	
addr [0 ... 254]	Show or set probe address.
Analog output	
amode	Show or set analog output mode (analog output limits and error level).
aover	Show or set analog output overrange and clipping behavior.
asel	Show or set analog output parameter and scaling.
Calibration and adjustment	
cco2	Adjust CO ₂ measurement gain and offset.
cdate	Show or set calibration date.
ct	Adjust temperature measurement offset.
ctext	Show or set calibration information.
Environmental compensation	
o2cmode	Show or set oxygen compensation mode.
pcmode	Show or set pressure compensation mode.
rhcmode	Show or set humidity compensation mode.
tcmode	Show or set temperature compensation mode.
Other commands	
frestore	Restore probe to factory settings.

4.9 Device Information and Status

Table 9 ? Command

Syntax	Description
?<cr>	Show listing of device information.
??<cr>	Show listing of device information even if device is in poll mode and connection has not been opened using the open command.

Syntax	Description
Example:	
<pre> ? Device : GMP25x Copyright : Copyright (c) Vaisala Oyj 2016. All rights reserved. SW Name : GMP25x SW version : 1.0.0 SNUM : GMP233_5_18 SSNUM : S1234567 CBNUM : c1234567 Calibrated : 20160504 @ Vaisala/R&D Address : 0 Smode : STOP </pre>	

Table 10 Errs Command

Syntax	Description
errs<cr>	Show active error(s). For a list of possible errors and their remedies, see Error Messages (page 99) .
Example (no active errors):	
<pre> errs NO CRITICAL ERRORS NO ERRORS NO WARNINGS STATUS NORMAL </pre>	

Table 11 Help Command

Syntax	Description
help<cr>	Show list of currently available serial commands.

Syntax	Description
Example (showing a list of the basic commands):	
<pre> help ADATE ADDR ATEXT CLOSE ENV ERRS FORM HELP INTV PASS RR ESET RX SDELAY SEND SENDX SERI SMODE SNUM SYSTEM UNIQID TIME VERS </pre>	

Table 12 Snum command

Syntax	Description
snum<cr>	Show serial number of the probe.
Example:	
<pre> snum SNUM : M0220028 </pre>	

Table 13 System Command

Syntax	Description
system<cr>	Show probe firmware information.

Syntax	Description
Example:	
<pre> system Device Name : GMP25x SW Name : GMP25x SW version : 1.0.0 Operating system : TSF0S1.0 </pre>	

Table 14 Time Command

Syntax	Description
time<cr>	Show how long the probe has been in operation since the last startup or reset. The operation counter is in format hh:mm:ss.
Example:	
<pre> time Time : 01:41:24 </pre>	

Table 15 Vers Command

Syntax	Description
vers<cr>	Show firmware version of the probe.
Example:	
<pre> vers SW version : 1.0.0 </pre>	

4.10 Serial Line Output and Communication

Table 16 Addr Command

Syntax	Description
addr<cr>	Show current device address. Addresses are required for POLL mode.

Syntax	Description
addr [aaa]<cr>	Set new device address. aaa = address, 0 ... 254 (default = 240)
Example (shows 0 as current address, enter 5 as the new address):	
<pre>addr Address : 0 addr 5 Address : 5</pre>	

Table 17 Close Command

Syntax	Description
close<cr>	Close the connection that was opened with the open command.
Example:	
<pre>close line closed</pre>	

Table 18 Form Command

Syntax	Description
form<cr>	Show the currently used measurement format.
form /<cr>	Reset measurement format to default.
form [sss]<cr>	Set a new measurement format. sss = String consisting of modifiers and abbreviations for measured parameters. See Table 19 on the facing page and Table 20 on the facing page. Maximum length is 150 characters. Maximum length may be shorter when text strings are used.

Syntax	Description
Example (show currently used measurement format (default format shown here)):	
<pre>form 6.0 "C02=" C02 " " U3 #r #n</pre>	
Output example (continuous output from RUN mode):	
<pre>C02= 452 ppm</pre>	
Example (set output format as %CO ₂):	
<pre>form 3.1 "C02=" C02% " " U4 #r #n OK</pre>	
Output example (continuous output from RUN mode):	
<pre>C02= 5.1 %C02 C02= 5.1 %C02 C02= 5.0 %C02 ...</pre>	
Example (set output format as CO ₂ ppm with Modulus-65536 checksum):	
<pre>form 6.0 "C02=" C02 " " U3 " " CS4 #r #n OK</pre>	
Output example (continuous output from RUN mode):	
<pre>C02= 3563 ppm 9F C02= 3562 ppm 9E C02= 3559 ppm A4 ...</pre>	

Syntax	Description
Example (set output format as CO ₂ ppm, with start of text (ASCII character 002) and end of text (003) ASCII codes, and without line feed and carriage return at the end):	
<pre>form #002 6.0 "CO2=" CO2 " " U3 #003 OK</pre>	
Output example (continuous output from RUN mode, ASCII codes not visible here):	
<pre>CO2= 866 ppm CO2= 866 ppm CO2= 867 ppm CO2= 867 ppm CO2= 867 ppm CO2= 868 ppm CO2= 868 ppm CO2= 869 ppm ...</pre>	

Table 19 Output Parameters for Form Command

Output Parameter	Abbreviation in Form Command
Carbon dioxide in ppm	co2
Carbon dioxide in percent	co2%
Currently used temperature compensation value	tcomp
Currently used pressure compensation value	pcomp
Currently used oxygen concentration compensation value	o2comp
Currently used relative humidity compensation value	rhcomp

Table 20 Modifiers for Form Command

Modifier	Description
x.y	Length modifier (number of digits and decimal places).
#t	Tabulator.
#r	Carriage-return.
#n	Line feed.
""	String constant, length 1 ... 15 characters.
#xxx	ASCII code value (decimal) of a special character; for example, #027 for ESC.
addr	Probe address (0 ... 254).
sn	Probe serial number.
time	Cumulative operating hours of the probe.

Modifier	Description
ux	Name of the measurement unit using x number of characters. For example, u3 shows the name of the measurement unit with three characters.
cs4	Modulus-65536 checksum of message sent so far, ASCII encoded hexadecimal notation.
csx	NMEA xor-checksum of message sent so far, ASCII encoded hexadecimal notation.



You can also use the backslash character \ instead of the hash character #.

Table 21 Intv Command

Syntax	Description
intv<cr>	Show the output interval of the automatically repeating measurement messages (r command and run mode).
intv [iii uuu]<cr>	Set the output interval. iii = interval, range 0 ... 255. u = unit for interval setting: <ul style="list-style-type: none"> • s = seconds • min = minutes • h = hours If you set the interval to 0, the output messages are output as quickly as they are generated, without additional delay.
Example:	
<pre>intv 5 s Output interval: 5 S</pre>	

Table 22 Open Command

Syntax	Description
open [aaa]<cr>	Open a connection to a device at the specified address. Required when device is in poll mode. aaa = address, range 0 ... 254.

Syntax	Description
Example (target probe in POLL mode, with address 52):	
<pre>open 52 GMP25x: 52 0pened for operator commands</pre>	

Table 23 R Command

Syntax	Description
r<cr>	Start the continuous outputting of measurement values as an ASCII text string to the serial line. The probe keeps outputting measurement messages at the interval that has been set with the intv command until stopped with the s command.
Example:	
<pre>r CO2= 1024 ppm CO2= 1024 ppm CO2= 1028 ppm CO2= 1026 ppm CO2= 1028 ppm ...</pre>	

Table 24 S Command

Syntax	Description
s<cr>	Stop the continuous outputting that was started with the r command.
Example:	
<pre>... CO2= 658 ppm CO2= 654 ppm CO2= 655 ppm s</pre>	

Table 25 Sdelay Command

Syntax	Description
sdelay<cr>	Show serial line transmission delay (1 ... 255). 1 unit = 4 milliseconds (for example, 5 = 0.020 second transmission delay).
sdelay [delay]<cr>	Set a new serial line transmission delay. delay = Serial line delay, range 1 ... 255 (1 unit = 4 ms).
Example (set delay to 0.1 seconds = 25 units):	
<pre>sdelay 25 COM transmit delay : 25</pre>	

Table 26 Send Command

Syntax	Description
send<cr>	Output a single measurement message.
send [aaa]<cr>	Output a single measurement message from a device in poll mode. aaa = address of the probe, range range 0 ... 254
Example:	
<pre>send C02= 1422 ppm</pre>	
Example (target probe in POLL mode, with address 52):	
<pre>send 52 C02= 458 ppm</pre>	

Table 27 Seri Command

Syntax	Description
seri<cr>	Show current serial line settings.

Syntax	Description
seri [b p d s]<cr>	<p>Set new serial line settings. The new settings will be taken into use when the probe is reset or powered up.</p> <p>b = baud rate (9600, 19200, or 38400)</p> <p>p = parity</p> <ul style="list-style-type: none"> • n = none • e = even • o = odd <p>d = data bits (7 or 8)</p> <p>s = stop bits (1 or 2)</p> <p>For Modbus, baud rate must be 9600 ... 38400 and parity must be none.</p>
<p>Example (show current settings):</p> <pre> seri Com1 Baud rate : 19200 Com1 Parity : N Com1 Data bits : 8 Com1 Stop bits : 1 </pre>	
<p>Example (set serial line to 9600 baud, even, 7 data bits, and 1 stop bit, and reset the probe to take the new settings in use):</p> <pre> seri 9600 e 7 1 OK seri Com1 Baud rate : 9600 Com1 Parity : E Com1 Data bits : 7 Com1 Stop bits : 1 reset GMP25x 1.0.0 </pre>	

Table 28 Smode Command

Syntax	Description
smode<cr>	Show current start-up operating mode of the serial line, and prompt to enter new mode.

Syntax	Description
smode [mode] <cr>	<p>Set serial line start-up operating mode. New mode is taken into use when the device is reset or powered up.</p> <p>Available modes:</p> <p>stop = No automatic output. All commands available. Default mode.</p> <p>run = Automatic output of measurement messages. You can stop the output with the s command, and recontinue with the r command.</p> <p>poll = No automatic output. Will respond to addressed send command and ?? command. You can use other commands after opening a connection using an addressed open command. Use with RS-485 buses where multiple probes can share the same line.</p> <p>modbus = Serial line communication uses the Modbus protocol. Serial line commands (Vaisala Industrial Protocol) are not accessible in the Modbus mode.</p> <p>analog = Switches the probe from digital output to analog output (active after probe reset). Serial line commands are not accessible in the analog mode.</p>
<p>Example (set serial mode to "poll"):</p> <pre>smode poll Serial mode : POLL</pre>	

4.11 Analog Output

Table 29 **Amode Command**

Syntax	Description
amode [channel] <cr>	<p>Show currently set analog output limits and error level.</p> <p>channel = Analog output channel</p> <ul style="list-style-type: none"> 1 = voltage output (V) 2 = current output (mA)


Syntax	Description
amode [channel lo_value hi_value error_value] <cr>	<p>Set new analog output limits and error output value.</p> <p>channel = Analog output channel</p> <ul style="list-style-type: none"> • 1 = voltage output (V) • 2 = current output (mA) <p>lo_value = Low limit of the channel.</p> <p>hi_value = High limit of the channel.</p> <p>error_value = Error value of the channel.</p> <div>  <p>When setting the error output voltage, note that the probe's maximum voltage output is 10.325 V.</p> </div>
<p>Example (show current configuration):</p> <pre> pass 1300 amode 1 Aout 1 range (V) : 0.00 ... 10.00 (error : 0.00) amode 2 Aout 2 range (mA) : 4.00 ... 20.00 (error : 2.00) </pre>	
<p>Example (set channel 1 to 0 ... 5 V, and error output to 0.0 V; set channel 2 to 0 ... 20 mA, and error output to 23 mA):</p> <pre> amode 1 0 5 0.0 Aout 1 range (V) : 0.00 ... 5.00 (error : 0.00) amode 2 0 20 23 Aout 2 range (mA) : 0.00 ... 20.00 (error : 23.00) </pre>	

Table 30 Aover Command

Syntax	Description
aover [channel] <cr>	<p>Show the behavior of the analog output when the measured value is outside the scaled output range.</p> <p>channel = Analog output channel</p> <ul style="list-style-type: none"> • 1 = voltage output (V) • 2 = current output (mA)

Syntax	Description
aover [channel clipping error_limit]<cr>	<p>Set the behavior of the analog output when the measured value is outside the scaled output range.</p> <p>channel = Analog output channel</p> <ul style="list-style-type: none">• 1 = voltage output (V)• 2 = current output (mA) <p>clipping = Output margin (%) at which the output is clipped.</p> <p>error_limit = Measurement value margin (%) at which the output of the channel goes into the error state. The current or voltage output of the error state is defined using the amode command.</p>
<p>Example (view currently set analog output overrange behavior on channel 1):</p> <pre>pass 1300 aover 1 Aout 1 clipping :5.00 % Aout 1 error limit :10.00 %</pre>	

Syntax	Description
<p>Example (for channel 1):</p> <ol style="list-style-type: none"> View currently set analog output scaling (asel command), limits and error level (amode command), and overrange behavior (aover command): <pre> pass 1300 asel 1 Aout 1 quantity : CO2(0 ... 2000) amode 1 Aout 1 range (V) : 0.00 ... 5.00 (error : 0.00) aover 1 Aout 1 clipping :1.00 % Aout 1 error limit :5.00 % </pre>	
<ol style="list-style-type: none"> Set analog output overrange clipping to 5 % and error limit to 10 %: <pre> aover 1 5 10 Aout 1 clipping : 5.00 % Aout 1 error limit : 10.00 % </pre>	
<p>The analog output now behaves like this:</p> <ul style="list-style-type: none"> Clipping is now set to 5.00 %, meaning the voltage output is allowed to vary between 0 ... 5.25 V. The analog channel will output the measurement for 0 ... 2100 ppmCO₂, but range 0 ... 5 V remains scaled to 0 ... 2000 ppmCO₂. Error limit is 10 %, which means the output will show the error state (0 V) when the measured CO₂ concentration is 10 % outside the scaled output range. With the settings above, this will happen if the measured CO₂ concentration is outside range 0 ... 2200 ppmCO₂. The voltage output will never be above 5.25 V because of clipping: the voltage output is clipped when the output reaches 5.25 V, and if the measured CO₂ concentration keeps rising above 2200 ppmCO₂, the output jumps directly to the error state 0 V. 	

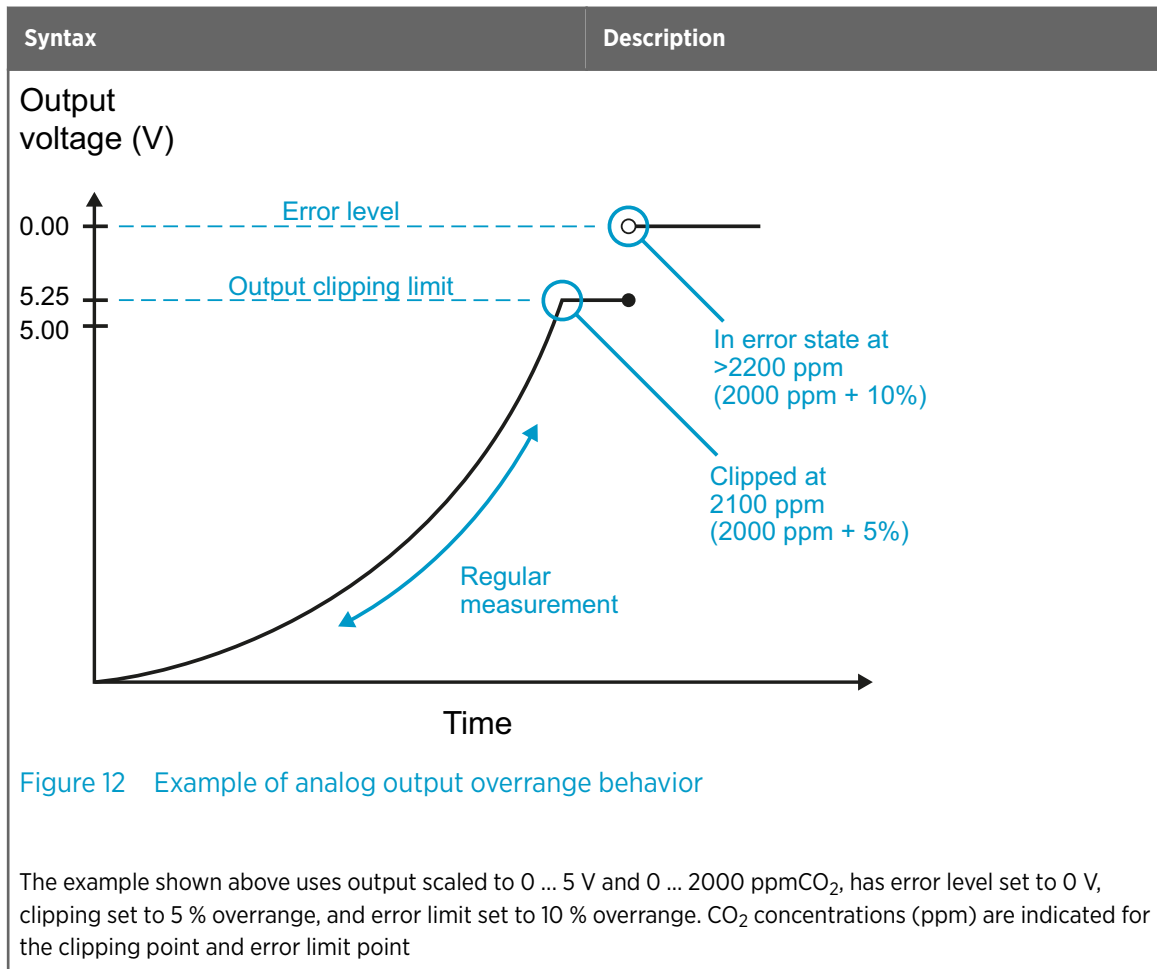


Table 31 AseI Command

Syntax	Description
asel [channel]<cr>	Show the parameter and scaling of the analog output in ppm. channel = Analog output channel <ul style="list-style-type: none"> • 1 = voltage output (V) • 2 = current output (mA)
asel [channel] [parameter lowlimit highlimit]<cr>	Set the parameter and scaling of the analog output. channel = Analog output channel parameter = Parameter that is output on analog channel. The only parameter available is CO ₂ (in ppm). lowlimit = Lower limit of channel scaling in ppm. Minimum value is -1000000 ppm (= - 100 %). highlimit = High limit of channel scaling in ppm. Maximum value is 1000000 ppm (= 100 %).

Syntax	Description
Example (for channel 1, show the currently set analog output parameter and scaling):	
<pre>pass 1300 asel 1 Aout 1 quantity : CO2(0 ... 10000 ppm)</pre>	
Example (for channel 1, set scaling to 0 ... 4000 ppmCO ₂):	
<pre>pass 1300 asel 1 co2 0 4000 Aout 1 quantity : CO2(0 ... 4000 ppm)</pre>	

4.12 Calibration and Adjustment



CAUTION! Before using the calibration and adjustment commands, read through [Calibration and Adjustment \(page 94\)](#). Make sure that the environmental compensation settings of the probe are properly set for your calibration environment; see [Environmental Compensation \(page 15\)](#).

Table 32 Adate Command

Syntax	Description
adate <cr>	Show CO ₂ factory adjustment date.
Example:	
<pre>adate Adjustment date : 20150420</pre>	

Table 33 Atext Command

Syntax	Description
atext <cr>	Show CO ₂ factory adjustment information.
Example:	
<pre>atext Adjusted at Vaisala/Helsinki</pre>	

Table 34 Cdate Command

Syntax	Description
cdate<cr>	Show calibration date.
cdate [yyyymmdd]<cr>	Set a new calibration date. yyyymmdd = Year (yyyy), month (mm) and day (dd) of calibration
Example:	
<pre>pass 1300 cdate Calibration date : 20150220</pre>	
Example (set a new calibration date to June 30, 2015):	
<pre>cdate 20150630 Calibration date : 20150630</pre>	

Table 35 Ctext Command

Syntax	Description
ctext<cr>	Show calibration information text.
ctext [text]<cr>	Set a new calibration information text to be shown after the automatic text "Calibrated at".
Example:	
<pre>pass 1300 ctext Calibrated at 500 ppm in lab</pre>	
Example (set a new information text):	
<pre>ctext 0/1000 by NN Calibrated at 0/1000 ppm by NN</pre>	

Table 36 CCO2 Command

Syntax	Description
cco2<cr>	Show current user adjustment status.

Syntax	Description
cco2 -lo [co2]<cr> cco2 -hi [co2]<cr>	Perform a 1-point (only either low or high concentration) or 2-point (both low and high concentrations) calibration and adjustment. -lo = Adjustment at low concentration (under 1000 ppmCO ₂) -hi = Adjustment at high concentration (over 2000 ppmCO ₂) co2 = CO ₂ concentration reference in ppm
cco2 -save<cr>	Save the currently entered adjustments. Successfully saving the adjustment clears the calibration date (cdate command) and calibration text (ctext command) that have been stored in the probe. Use those commands to enter a new calibration date and text.
cco2 -cancel<cr>	Cancel currently entered adjustments.
cco2 -reset<cr>	Clear user adjustments.
Example (show current user adjustment status; no adjustment done): <pre> pass 1300 cco2 1.Ref. point low 0 1.Meas. point low 0 2.Ref. point high 3000 2.Meas. point high 3000 Gain : 1.0000 Offset : 0.0000 </pre>	
Example (perform a 1-point calibration): <ol style="list-style-type: none"> Let the probe stabilize in the desired CO₂ concentration (here: 500 ppmCO₂). Enter the calibration commands: <pre> pass 1300 cco2 -lo 500 OK cco2 -save OK </pre> Enter a new calibration date and information text: <pre> cdate 20160325 Calibration date : 20160325 ctext 500 ppm in lab Calibrated at 500 ppm in lab </pre> 	

Syntax	Description
<p>Example (perform 2-point calibration):</p> <ol style="list-style-type: none"> 1. Let the probe stabilize in the desired low CO₂ concentration (here: 200 ppmCO₂). 2. Enter the calibration commands: <pre>pass 1300 cco2 -lo 200 OK cco2 -save OK</pre> <ol style="list-style-type: none"> 3. Let the probe stabilize in the desired high CO₂ concentration (here: 3000 ppmCO₂). 4. Enter the calibration commands: <pre>pass 1300 cco2 -hi 3000 OK cco2 -save OK</pre> <ol style="list-style-type: none"> 5. Enter a new calibration date and information text: <pre>pass 1300 cdate 20160425 Calibration date : 20160425 ctext 200/3000 ppm Calibrated at 200/3000 ppm</pre>	

4.13 Environmental Compensation Commands




To apply an accurate relative humidity compensation, the temperature and pressure compensation configurations must also match your measurement environment. See the **rhcmode**, **tcmode** and **pcmode** commands for instructions on enabling compensation configuration, and **env** command for instructions on setting a compensation value.



For more information on environmental compensation and the default (neutral) compensation values used for disabled compensations, see [Environmental Compensation \(page 15\)](#)

Table 37 Env Command

Syntax	Description
env<cr>	<p>Show current compensation values.</p> <p>Before using this command, you must enable environmental compensation using the following commands:</p> <ul style="list-style-type: none"> • o2cmode [on] • pcmode [on] • rhcmode [on] • tcmode [on measured]
env [temp pres oxy hum] [value]<cr>	<p>Set new permanent compensation values and store them in eeeprom.</p> <p>Eeprom:</p> <ul style="list-style-type: none"> • Non-volatile memory, values retained during power off. • Number of writes is limited to 30000 cycles by memory implementation. • Must only be used for writing permanent values, to avoid wearing out the eeprom. <p>temp = Compensation temperature. Range -40 ... +100 °C.</p> <p>pres = Compensation pressure. Range 500 ... 1100 hPa.</p> <p>oxy = Oxygen content of background gas. Range 0 ... 100 %.</p> <p>hum = Relative humidity of background gas. Range 0 ... 100 %.</p>

Syntax	Description
env [xtemp xpres xoxy xhum] [value]<cr>	<p>Set new compensation values and store them in RAM.</p> <p>RAM: n Volatile memory that loses the values when probe is reset, and where values are loaded from non-volatile memory at startup. n Must be used for continuously updated values.</p> <p>xtemp = Compensation temperature stored in RAM. Range -40 ... 100 °C.</p> <p>xpres = Compensation pressure stored in RAM. Range 500 ... 1100 hPa.</p> <p>xoxy = Oxygen content of background gas stored in RAM. Range 0 ... 100 %.</p> <p>xhum = Relative humidity of background gas stored in RAM. Range 0 ... 100 %.</p> <div>  <p>Note: If temperature compensation is configured to use an internally measured value (tcmode is set to measured), it will continuously update the value in RAM, overriding any temperature value that is written to RAM with the ENV command.</p> </div>
<p>Example (Show current compensation values; all compensations are enabled. Note that temperature compensation is in "measured" mode, so the value in use is constantly changing):</p> <pre> env In eeprom: Temperature (C) : 8.00 Pressure (hPa) : 1013.00 Oxygen (%O2) : 21.00 Humidity (%RH) : 30.00 In use: Temperature (C) : 4.90 Pressure (hPa) : 1013.00 Oxygen (%O2) : 19.70 Humidity (%RH) : 27.00 </pre>	

Syntax	Description
Example (set temperature compensation to setpoint mode, and change temperature setpoint value to 5.00 °C in RAM):	
<pre> pass 1300 tcmode on T COMP MODE : ON env xtemp 5.00 In eeprom: Temperature (C) : 8.00 Pressure (hPa) : 1013.00 Oxygen (%O2) : 21.00 Humidity (%RH) : 30.000 In use: Temperature (C) : 5.00 Pressure (hPa) : 1013.00 Oxygen (%O2) : 21.00 Humidity (%RH) : 30.00 </pre>	


Table 38 O2cmode Command

Syntax	Description
o2cmode<cr>	Check current oxygen compensation mode. Possible modes: <ul style="list-style-type: none"> • on = Compensation enabled using setpoint value. • off = Compensation disabled, default (neutral) value used: see Environmental Compensation (page 15)
o2cmode [on off]<cr>	Change oxygen compensation mode (on or off).
Example (check oxygen compensation mode; oxygen compensation is disabled, a neutral value is used):	
<pre> pass 1300 o2cmode O2 COMP MODE : OFF </pre>	
Example (enable oxygen compensation):	
<pre> pass 1300 o2cmode on O2 COMP MODE : ON </pre>	

Table 39 Pcmode Command

Syntax	Description
pcmode<cr>	Check current pressure compensation mode. Possible modes: <ul style="list-style-type: none"> • on = Compensation enabled using setpoint value. • off = Compensation disabled, default (neutral) value used: see Environmental Compensation (page 15).
pcmode [on off]<cr>	Change pressure compensation mode (on or off).
Example (check pressure compensation mode; pressure compensation is enabled using a setpoint value):	
<pre>pass 1300 pcmode P COMP MODE : ON</pre>	

Table 40 Rhcmode Command

Syntax	Description
rhcmode<cr>	Check current relative humidity compensation mode. Possible modes: <ul style="list-style-type: none"> • on = Compensation enabled using setpoint value. • off = Compensation disabled, default (neutral) value used: see Environmental Compensation (page 15). <div>  <p>To apply an accurate relative humidity compensation, make sure that the temperature compensation and pressure compensation configurations also match the measurement environment.</p> </div>
rhcmode [on off]<cr>	Change relative humidity compensation mode (on or off).
Example (check relative humidity compensation mode; relative humidity compensation is disabled, a neutral value is used):	
<pre>pass 1300 rhcmode RH COMP MODE : OFF</pre>	

Syntax	Description
Example (enable temperature, pressure and relative humidity compensation using setpoint values):	
<pre> pass 1300 tcmode on T COMP MODE : ON pcmode on P COMP MODE : ON rhcmode on RH COMP MODE : ON </pre>	

Table 41 Tcmode Command

Syntax	Description
tcmode<cr>	Check current temperature compensation mode. Possible modes: <ul style="list-style-type: none"> • on = Compensation enabled using setpoint value. • off = Compensation disabled, default (neutral) value used: see Environmental Compensation (page 15) • measured = Compensation enabled using internal measurement.
tcmode [on off measured]<cr>	Change temperature compensation mode (on , off or measured).
Example (check temperature compensation mode; temperature compensation is enabled using a setpoint value):	
<pre> pass 1300 tcmode T COMP MODE : ON </pre>	
Example (change temperature compensation to use internal measurement):	
<pre> pass 1300 tcmode measured T COMP MODE : MEASURED </pre>	

4.14 Other Commands

Table 42 Frestore Command


Syntax	Description
frestore <cr>	<p>Restore the probe to its factory configuration. All user settings and user calibration parameters will be lost.</p> <div>  <p>After using the frestore command, reset the probe using the reset command.</p> </div>
<p>Example (restore the factory settings and reset the probe):</p> <pre> pass 1300 frestore Parameters restored to factory defaults reset GMP25x 1.0.0 </pre>	

Table 43 Pass Command

Syntax	Description
pass [code]<cr>	<p>Access advanced serial commands.</p> <p>Advanced commands can be used until the next reset.</p> <p>code = Code for enabling advanced commands (1300).</p>
<p>Example:</p> <pre> pass 1300 </pre>	

Table 44 Reset Command

Syntax	Description
reset <cr>	<p>Reset the probe. The probe will restart as if it had just been powered on.</p>
<p>Example:</p> <pre> reset GMP25x 1.0.0 </pre>	

5. Modbus

The probe can be accessed using the Modbus serial communication protocol. The supported Modbus variant is Modbus RTU (Serial Modbus) over RS-485 interface.

For instructions on enabling the Modbus mode when you are using the probe with Vaisala Industrial Protocol, see [Enabling Modbus Mode from Vaisala Industrial Protocol \(page 30\)](#).

For instructions on switching to Vaisala Industrial Protocol when the probe is in Modbus mode, see [Accessing Serial Commands from Modbus or Analog Mode \(page 30\)](#).

For information on using Modbus with the Indigo 202 digital transmitter, see [Using Modbus with Indigo 202 \(page 73\)](#).

The pre-configured default Modbus serial settings are presented in the following table.

Table 45 Default Modbus Serial Communication Settings

Description	Default Value
Serial bit rate	19200
Parity	N
Number of data bits	8
Number of stop bits	2
Modbus device address	240

More Information

- [Function Codes \(page 113\)](#)
- [Modbus Registers \(page 113\)](#)

6. Vaisala Insight Software

Vaisala Insight software is a configuration software for Indigo-compatible probes. The supported operating systems are Windows 7 (64-bit), Windows 8.1 (64-bit), and Windows 10 (64-bit).

With the Insight software, you can:

- See device information and status.
- See real-time measurement.
- Configure serial communication settings, purge settings, filtering factor, and analog output parameters and scaling.
- Calibrate and adjust the device.

Download Vaisala Insight software at www.vaisala.com/insight.

The probe can be connected to Vaisala Insight software using a Vaisala USB cable (no. 242659).



GMP252 probes support Insight from probe software version 1.3.0 onwards.

6.1 Connecting to Insight Software



- Computer with Vaisala Insight software installed
- USB connection cable (no. 242659)

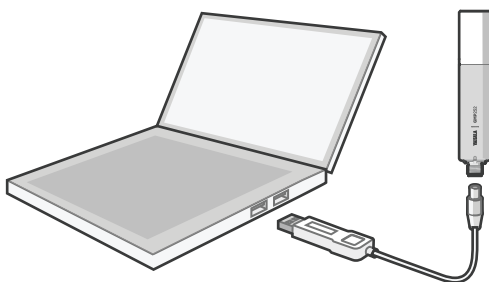


Figure 13 Connecting Probe to Insight



Connect the probe to the Insight software in the exact order described in the following steps.

- ▶ 1. Open the Insight software.
- 2. Connect the USB cable to a free USB port on the PC.
- 3. Connect the probe to the USB cable.
- 4. Wait for Insight software to detect the probe.

7. Using GMP252 with Indigo Transmitters

7.1 Indigo Overview

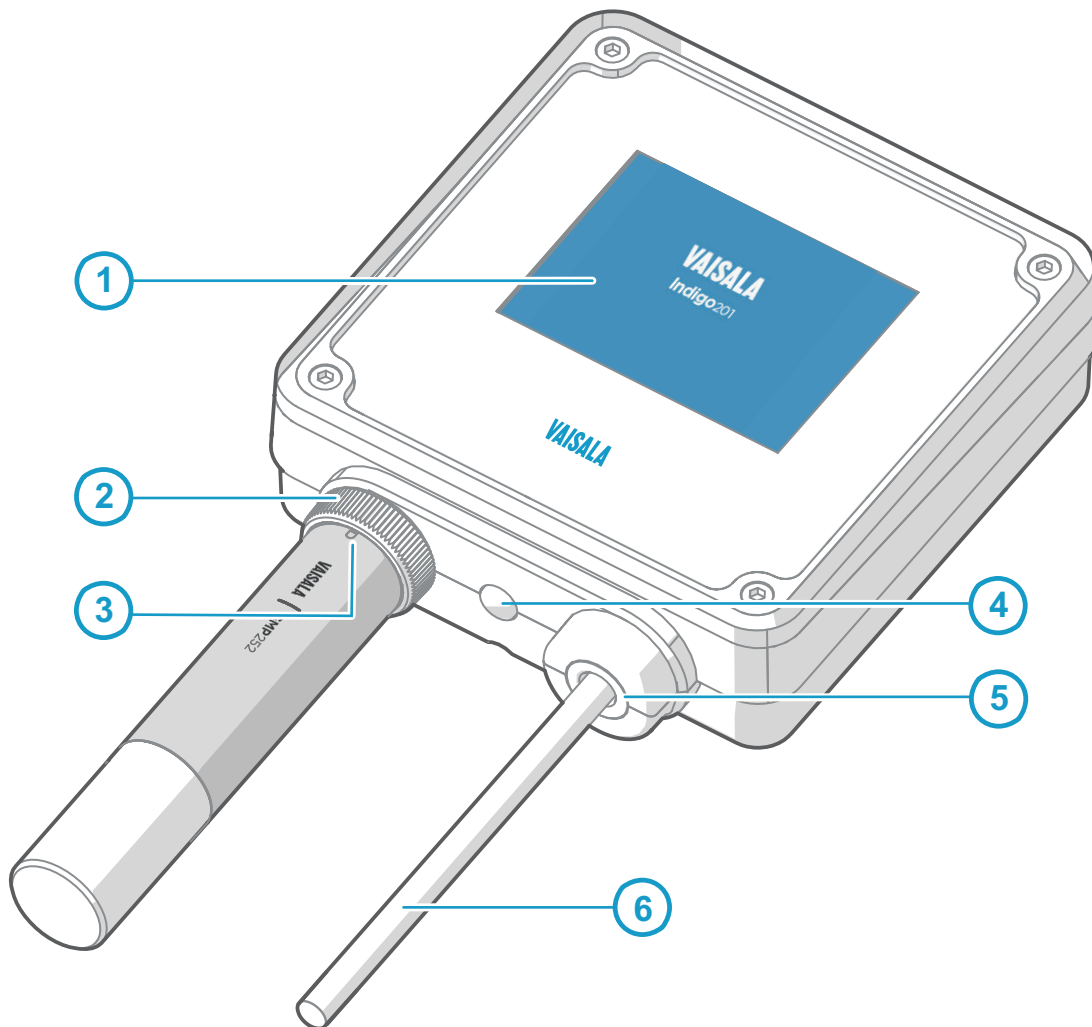


Figure 14 GMP252 Attached to Indigo Transmitter

- 1 3.5" TFT LCD color display: non-display option with LED available for certain models.
- 2 Probe locking wheel: insert probe, hold in place and turn the wheel counterclockwise.
- 3 Probe orientation mark: insert the probe with the orientation mark facing out.
- 4 Wireless configuration interface (WLAN) activation button.
- 5 Rubber lead-through with strain relief. Cable feedthrough option also at back of transmitter.
- 6 Input/output cable.

The probe can be connected to Vaisala Indigo transmitters, either directly on the transmitter from the probe's connector, or by using a cable between Indigo and the probe.

Indigo transmitters are host devices that extend the feature set of connected probes with a range of additional options for outputs, configuration access, measurement viewing, and status monitoring.

The selection of available additional features (for example, output and connectivity options) varies depending on the Indigo transmitter model. Depending on the model, a display is available as an optional selection or as a standard feature. In the non-display model, an LED indicator is used for notifications.

7.1.1 Wireless Configuration Interface Overview

Indigo transmitters are configured using a wireless browser-based configuration interface (requires a mobile device or computer with IEEE 802.11 b/g/n WLAN wireless connectivity). In addition to probe and transmitter configuration and calibration, you can also use the wireless interface to view measurement data and status information.



Figure 15 Desktop and Mobile Example Views

The wireless configuration interface has two user levels:

- All users have view-only access (no configuration rights, not password protected).
- Personnel that carry out configuration tasks can log in with an administrative password that allows changing the transmitter and probe settings.

To use the wireless configuration interface to modify the settings of your Indigo transmitter and the connected probe, you must first enable the transmitter's wireless connection and then connect to Indigo with your mobile device or computer. Most major browsers (for example, Firefox, Chrome, Safari, and Internet Explorer) are supported: using the most recent version is recommended.

7.2 Taking a Probe in Use with Indigo

In order to use the probe with an Indigo transmitter, you need to connect the probe to an Indigo transmitter and use a mobile device or computer to review the transmitter and probe configuration with Indigo's wireless configuration interface.



- Indigo-compatible probe and Indigo transmitter
- Mobile device or computer that supports wireless connectivity (IEEE 802.11 b/g/n WLAN)
- Web browser

To take the probe in use with Indigo:

1. Connect the probe to a wired and powered Indigo transmitter and check that the transmitter recognizes the probe (green LED/display notification).
2. Enable Indigo's wireless connection and open the Indigo wireless configuration interface in your mobile device or computer.
3. Use Indigo's wireless configuration interface to check that the probe and transmitter settings are correct for your system. For instructions on using the wireless configuration interface, see the *User Guide* of the Indigo transmitter.

More Information

- [Attaching Probes and Cables \(page 67\)](#)
- [Connecting to Wireless Configuration Interface \(page 68\)](#)
- [Wireless Interface Menus \(page 70\)](#)
- [Logging in to Wireless Configuration Interface \(page 69\)](#)

7.2.1 Checking Indigo Support in Probe

To verify that your probe supports Indigo, check the serial number on the probe body. All probes intended for use with Indigo manufactured from 2017 onwards (serial numbers starting with the letter **N** or latter in alphabetical order) are compatible with Indigo.



Figure 16 Serial Number on Probe Body (GMP251 Example)

- 1 Probes with a serial number starting with the letter **N** have been manufactured in 2017.

7.3 Attaching Probes and Cables

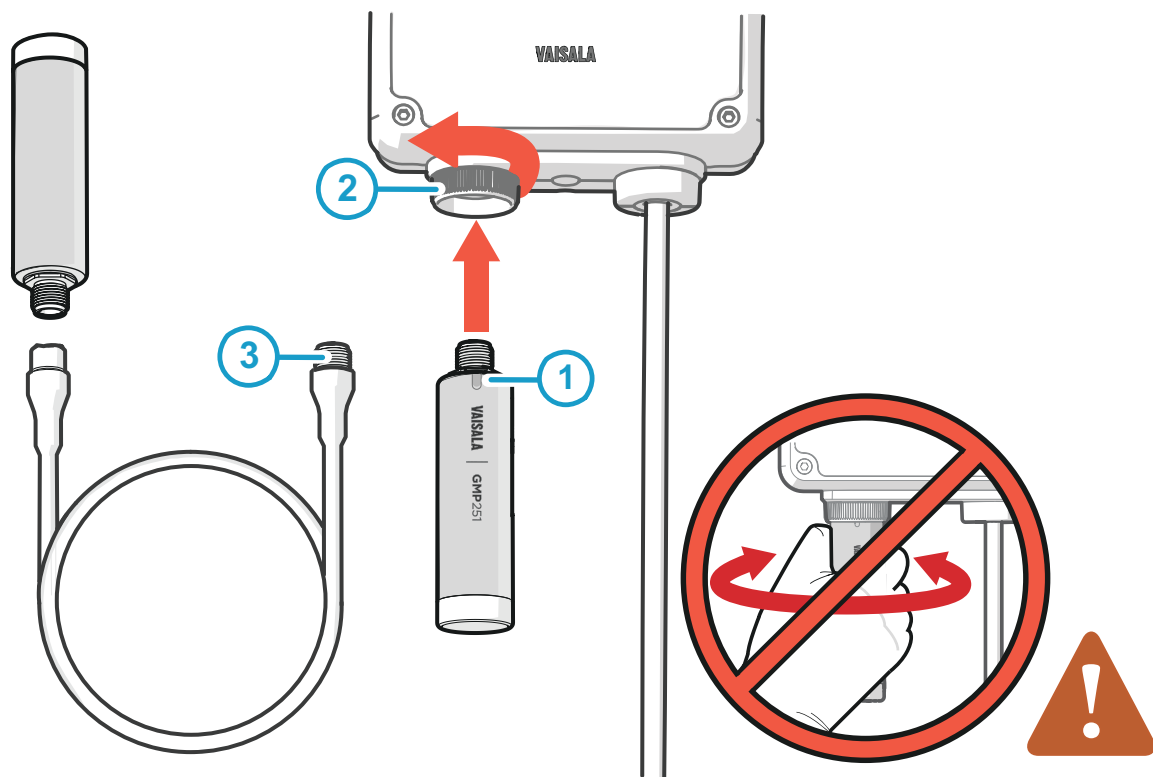


Figure 17 Attaching Probes and Cables to Indigo

- 1 Insert probes into the probe connector with the orientation mark facing out.
- 2 Probes are locked in place with the locking wheel. **Never turn from the probe body.**
- 3 Connect probe cables in the same way as probes: insert the cable in the connector and hold in place while turning the locking wheel.

- ▶ 1. Insert the probe into the probe connector with the orientation mark on the probe body facing out.
- 2. Hold the probe in the probe connector and lock it in place by turning the locking wheel counterclockwise. Never turn the probe body when attaching or removing probes, only the locking wheel of the Indigo transmitter.
- 3. When the transmitter recognizes the connected probe, it shows a notification message on the display (for example, **Probe Connected: GMP251**). In the non-display model, a green LED is lit when Indigo recognizes the probe.

7.4 Connecting to Wireless Configuration Interface

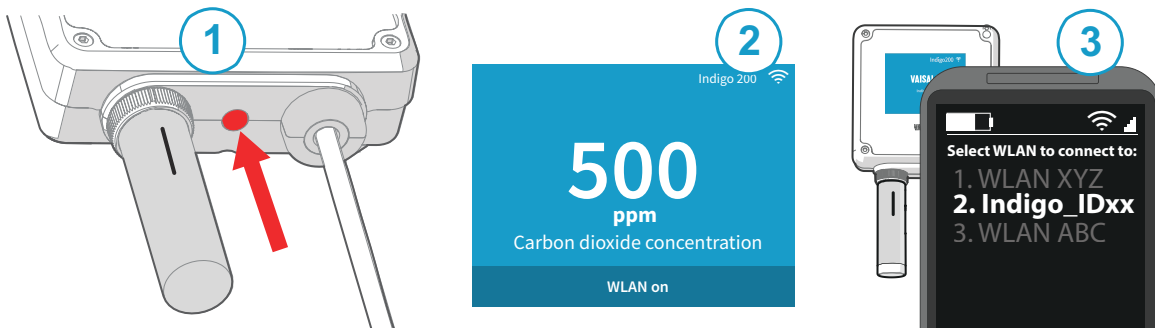


Figure 18 Enabling and Accessing Indigo's Wireless Configuration Interface

- 1 Wireless connection activation button
- 2 Wireless connection indicator (WLAN symbol) on the Indigo display
- 3 Choose Indigo (**Indigo_ID[xx]**) from your wireless device's list of available connections

To connect to the wireless configuration interface:

- ▶ 1. Press the wireless connection activation button on the bottom of the transmitter.
2. When the wireless configuration interface becomes available, the Indigo display shows a connection notification. In the Indigo models with an LED indicator, the LED blinks green when the connection is active.
3. Open the wireless connection menu in your mobile device or computer and select **Indigo_ID[xx]** (transmitter-specific SSID) from the list of available connections.
4. Depending on your device, the wireless configuration interface either launches automatically in your browser after you connect to Indigo, or you may need to start your browser application manually.
5. When you open the Indigo interface in your browser, you are prompted to log in.



Only one device can be connected to the wireless configuration interface at a time.

More Information

- ▶ [Logging in to Wireless Configuration Interface \(page 69\)](#)
- ▶ [Wireless Interface Menus \(page 70\)](#)

7.5 Logging in to Wireless Configuration Interface

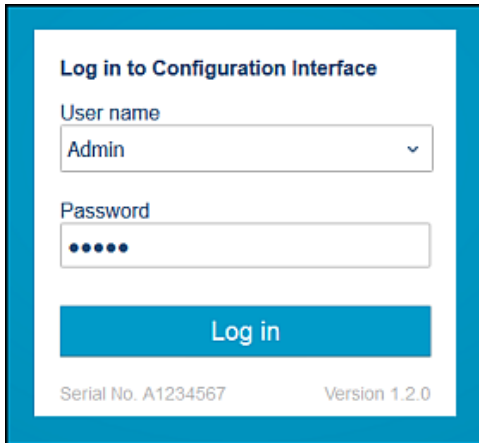


Figure 19 Indigo Login View

When you open Indigo's wireless configuration interface in your browser, you are prompted to log in. There are 2 available user levels:

- **User:** view-only access available for all users. Does not require a password.
- **Admin:** password-protected access. To change settings, you must log in as admin.

To log in:

1. Enter the user name and password:
 - a. To log in as user (view-only access, no configuration rights), select **User** from the **User name** dropdown. Leave the **Password** field empty.
 - b. To log in as admin (required for configuration), select **Admin** in the **User name** dropdown and type the admin password (default: **12345**) in the **Password** field.
2. Select **Log in** after entering the login credentials. The wireless configuration interface opens in the **Measurements** view.



The user level (**User** or **Admin**) is shown in the upper right corner of all menu views. Select the user/admin icon in the upper right corner to change the user level.

7.6 Wireless Interface Menus

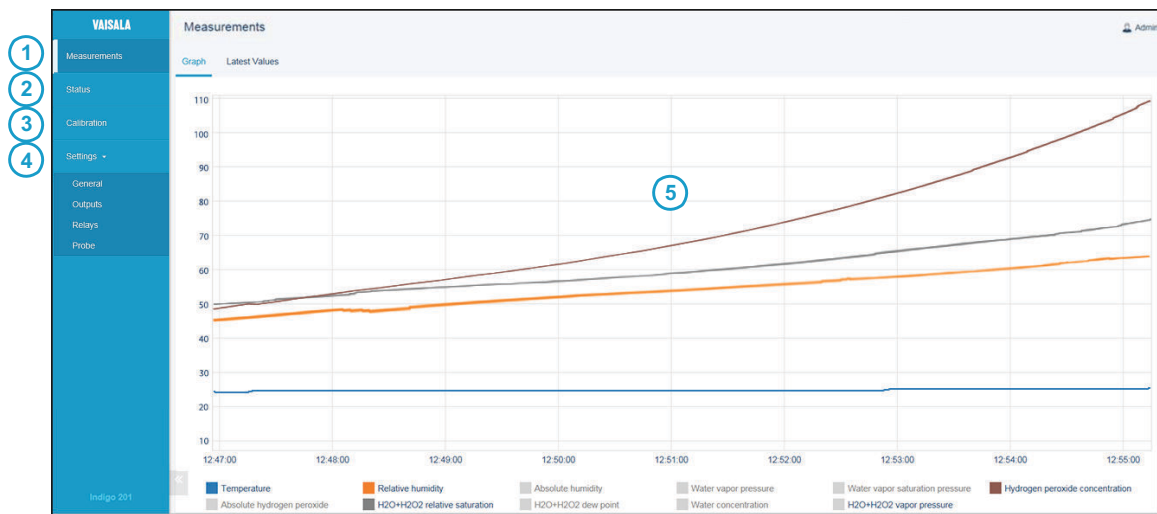


Figure 20 Wireless Configuration Interface, Desktop Browser View

- 1 **Measurements:** displays the measurement data of the connected probe
- 2 **Status:** contains information about the status of Indigo and the connected probe (for example, notifications and alarms)
- 3 **Calibration:** calibrate and adjust probes using references. Available options (for example, adjustment points) vary depending on the probe model.
- 4 **Settings:** contains options for configuring the connection and display settings, outputs, relays, probe-specific settings, and general device preferences
 - **General** submenu: device information and general settings, wireless connection and display settings
 - **Outputs** submenu: options for configuring analog or digital outputs (depending on transmitter model).
 - **Relays** submenu: settings for controlling relays A and B
 - **Probe** submenu: probe-specific settings such as environmental compensations and filtering factor
- 5 Main display area for menus and measurement information (desktop browser example)



For more information on the configuration options available in Indigo transmitters, see the *User Guide* of your transmitter.

7.7 Configuring Analog Outputs with Indigo 201

Indigo 201 analog output transmitters have 3 analog current (mA) or voltage (V) outputs. Each analog output has the same set of configuration options (analog output 1 shown in example).

Note that you must select either the current or voltage output mode: using both current and voltage outputs is not possible.



When you enter a value into a field, the value is saved automatically when you exit the input field (for example, tap on an area outside of the field).

General

Mode

Analog Output 1

Output Type

Parameter

Unit

Scale Low End

Scale High End

Clipping Limit %

Error Limit %

Error Output Voltage

Error Output Current

Figure 21 Indigo 201 Analog Output Configuration Options



For detailed instructions on configuring analog outputs in the Indigo 201 wireless configuration interface, see *Indigo 201 Analog Output Transmitter User Guide*.

More Information

- [Indigo 201 Analog Output Mode Selection \(page 72\)](#)

7.7.1 Receiving Analog Output Settings from Probe

When you take Indigo 201 in use for the first time and have not entered an analog output configuration, the transmitter automatically adapts the analog output configuration of the first Vaisala Indigo-compatible probe you connect.

If an analog output configuration already exists in Indigo 201 (that is, you have previously connected a probe or configured the settings), you need to set the analog output configuration of the new probe manually. Analog output from the transmitter is halted and does not resume until you have set the new probe's configuration.

Alternatively, you can clear the analog output settings in Indigo 201 configuration. This returns the transmitter to a state where it automatically starts using the analog output configuration of the next connected probe. The analog output settings can be cleared from the **Settings > General** menu.

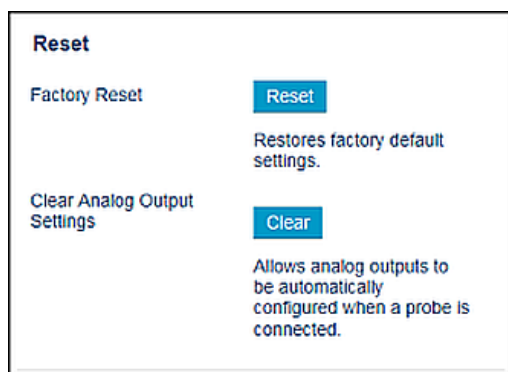


Figure 22 Clearing Analog Output Settings

7.7.2 Indigo 201 Analog Output Mode Selection

Indigo 201 has 3 analog output channels for either current (mA) or voltage (V) output. All 3 channels must use the same output mode (mA or V): it is not possible to use both voltage and current outputs simultaneously.

The output mode selection is made in the **Settings > Outputs** menu of the wireless configuration interface.

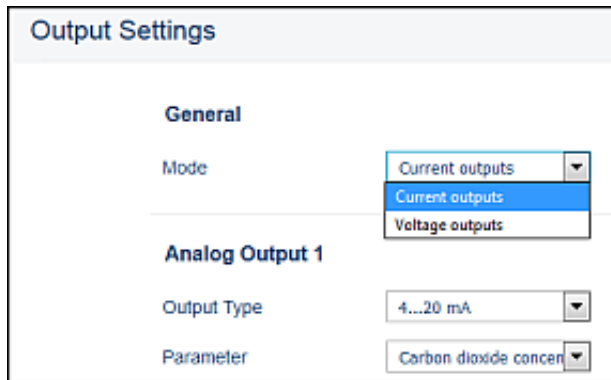


Figure 23 Selecting Indigo 201 Analog Output Mode

7.8 Using Modbus with Indigo 202

Indigo 202 digital transmitters are designed for Modbus RTU (RS-485) communication. There are 2 groups of Modbus register addresses in use in Indigo 202: probe registers and Indigo registers. The probe registers are received from the connected probe, and are organized according to the probe's register map. Indigo registers include transmitter-specific information.

Received Modbus requests for register operations are treated in two different ways depending on the register address. Addresses above $DFFF_{\text{hex}}$ (that is, Indigo registers) are handled as normal requests. Lower addresses (that is, probe registers 0000_{hex} ... $DFFF_{\text{hex}}$) are passed to the measurement probe, and the response from the probe is again passed to original Modbus client. Indigo can also have a cache for commonly requested registers (Measurement registers).

The maximum response delay is 2 seconds (when data content needs to be fetched from the probe). The minimum delay between requests is 10 ms.



For more details on the information relayed within Indigo 202 (transmitter-specific) Modbus registers, see *Indigo 202 Digital Transmitter User Guide*.

Table 46 Indigo 202 Modbus Registers

Address	Name	Data Type
Probe registers (according to the connected probe's register map) ¹⁾		
0000_{hex}	First measurement probe address	
$DFFF_{\text{hex}}$	Last measurement probe address	
Indigo registers		
$E000_{\text{hex}}$	Status	16-bit
$E001_{\text{hex}}$	Notification and error bits	16-bit

Address	Name	Data Type
E002 _{hex}	Connected probe	text [30]
E011 _{hex}	Relay A status	enum
E012 _{hex}	Relay B status	enum

1) See the connected probe's Modbus documentation for probe-specific register information

More Information

- [Modbus Registers \(page 113\)](#)
- [Modbus \(page 59\)](#)

7.8.1 Modbus Serial Communication Settings

The **Settings > Outputs** menu of the wireless configuration interface contains the configuration options for Modbus serial communication.

Serial Communication

Protocol
Modbus RTU

Speed
19200

Stop Bits
2

Parity
NONE

Modbus

Slave Address
10

[Protocol](#)
[Speed](#)

Modbus protocol options. The **Modbus RTU** protocol is in use by default. Select the baud rate used in Modbus communication: **4800**, **9600**, **19200**, **38400**, **57600**, or **115200**. Default: **19200**.

[Stop Bits](#)
[Parity](#)

Stop bits used in Modbus communication: **1** or **2**. Default: **2**.
Select **EVEN**, **ODD** or **NONE**. Default: **NONE**.

[Slave Address](#)

Address used when Indigo functions as a Modbus slave (range: **1 ... 247**). Default: **10**.

7.9 Configuring Relays with Indigo

Indigo transmitters have 2 configurable relays (relay A and relay B). Both relays have configuration options for selecting the parameter that is used to control the relay, activation triggers, hysteresis, and error state behavior.

Relay A	
Output Mode	Active above trigger level 1
Parameter	Carbon dioxide concentra 2
Unit	% 3
Low Trigger Level	1.00 4
High Trigger Level	2.00 4
Error State	Inactive 5

Figure 24 Relay Configuration Options

- 1 **Output Mode:** Select whether the relay activates above or below a set trigger value (or set the relay **Off**).
- 2 **Parameter:** The measurement that is used to control the relay.
- 3 **Unit:** Select the unit of the measurement parameter that controls the relay (for example, % if the measurement is in %CO₂).
- 4 **Low Trigger Level** and **High Trigger Level:** If you want to activate the relay above or below a single setpoint without using hysteresis, enter the same value for the low trigger and the high trigger. The **Output Mode** selection defines whether the relay activates above or below this value.
If you want to set a hysteresis, define the limits of the hysteresis with the low and high triggers. See the Indigo documentation for instructions on setting a hysteresis.
- 5 **Error State:** Select which state the relay is set to when an error occurs (on, off, or remains in its current state)



For detailed instructions on configuring relays with Indigo, see the Indigo transmitter's *User Guide*.

7.10 Changing Environmental Compensation Settings with Indigo

The configuration options in Indigo transmitters include probe-specific settings that vary depending on the features of the connected probe.

In the case of Vaisala CARBOCAP® Carbon Dioxide Probes GMP251 and GMP252, the probe-specific settings allow configuring the filtering factor and environmental compensations.

To change the environmental compensation settings:

1. Launch the Indigo wireless configuration interface and open the **Settings > Probe** menu.
2. Enable the required environmental compensations (set the compensation **On** or **Off**) you need to use in the **Measurement** selections. For temperature compensation, select either the measurement from the probe sensor (**Measured**), or manual **Setpoint** entry.

Pressure compensation on/off	<input type="text" value="On"/>
Temperature compensation mode	<input type="text" value="Setpoint"/>
Humidity compensation on/off	<input type="text" value="Off"/>
Oxygen compensation on/off	<input type="text" value="Off"/>

3. Enter the setpoint values for the compensations you have enabled into the **Compensation setpoints** text fields.



The values entered into the **Compensation setpoints** fields are only for temporary use: when you reset the probe, the default values (see **Compensation power-up defaults**) are restored.

Compensation setpoints	
Temperature	<input type="text" value="25.00"/>
Relative humidity	<input type="text" value="0.00"/>
Pressure	<input type="text" value="1013.00"/>
Oxygen concentration	<input type="text" value="0.00"/>

4. Enter the power-up default compensation values that are stored into the probe's permanent memory.

Compensation power-up defaults	
Temperature	<input type="text" value="25.00"/>
Relative humidity	<input type="text" value="0.00"/>
Pressure	<input type="text" value="1013.00"/>
Oxygen concentration	<input type="text" value="0.00"/>



The values entered into the **Compensation power-up defaults** fields remain in use also after probe reset.

5. The values you enter are saved automatically when you exit the input field (for example, tap on an area outside of the field).



Note that the environmental compensations you set in the **Settings > Probe** and the compensations set on the **Configuration** tab of the **Calibration** menu are interconnected: the configuration set in either menu is applied to both.

More Information

- [Environmental Compensation \(page 15\)](#)

7.11 Configuring Filtering Factor with Indigo

Measurement	
Filtering factor	<input type="text" value="100"/>

The filtering factor affects the speed at which the latest measurement is integrated into the output of the probe: a new measurement is produced approximately every two seconds. You can configure the filtering factor in the **Settings > Probe** menu of Indigo's wireless configuration interface.

By default, the filtering factor is set to 1.0 (1.0 = 100 in the configuration range), which means the latest measurement is shown directly in the output, without any filtering. To apply filtering, enter a lower filtering factor to include previous measurements in the calculation of measurement output. For example, changing the filtering factor to 0.1 results in an output that is a combination of previous measurements (90%) and the latest measurement (10%).

The configuration range of the filtering factor is 0 ... 100: for example, to set the factor to 0.5, set the value to 50.

More Information

- [Filtering Factor \(page 120\)](#)

7.12 Calibrating GMP252 with Indigo

7.12.1 Indigo Calibration Overview

You can carry out 1-point and 2-point adjustments with the Indigo transmitter's wireless configuration interface. In addition to calibrating and adjusting probes, you can view the current adjustments and restore the probe's factory adjustment.

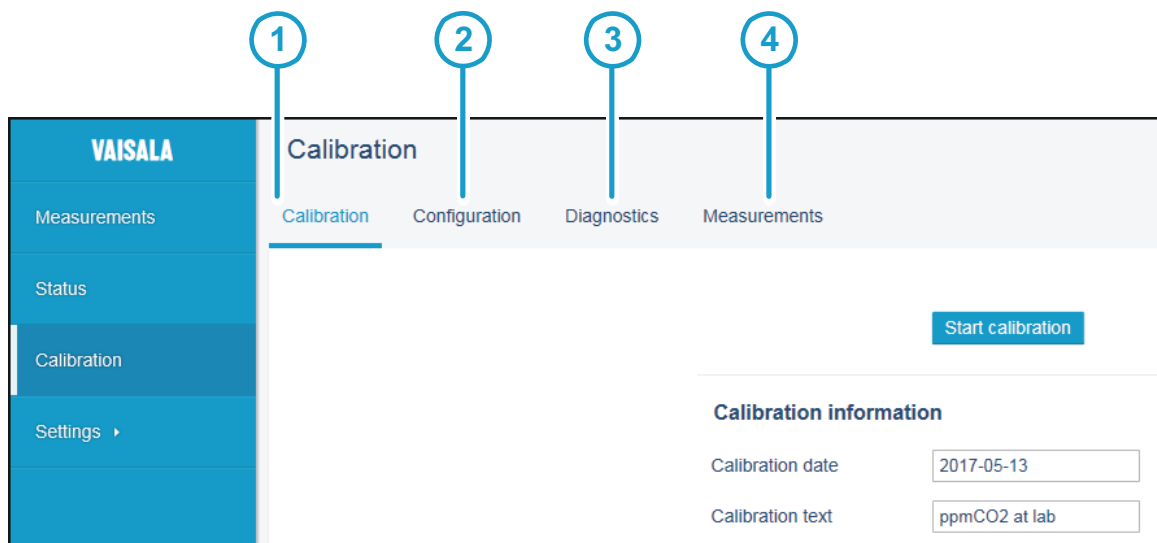


Figure 25 Calibration Menu Main View

- 1 Calibration tab
- 2 Configuration tab
- 3 Diagnostics tab
- 4 Measurements tab

There are 4 tabs in the **Calibration** menu:

- **Calibration:** the main adjustment view with options for making adjustments, viewing adjustments, and restoring factory adjustments.

- **Configuration:** options for using environmental compensations (probe-specific range of options) that allow compensating for the conditions present in the calibration environment, for example, pressure, temperature, and background gases. Also includes probe-specific configuration options that are not mandatory for use with Indigo.
- **Diagnostics:** this tab contains information about the status of the measurement and the probe, and shows the current environmental compensation configuration.
- **Measurements:** this tab shows the current probe measurement in numeric format (use this view, for example, when you need to follow measurement stabilization in a reference environment without leaving the **Calibration** menu).



Before adjusting the probe's measurement, make sure you have gone through the information in [Calibration and Adjustment \(page 94\)](#).

Starting and Closing Calibration Mode in Indigo

In order to be able to use the calibration options, you must switch the operation of the probe and Indigo to calibration mode with the **Start calibration** button.

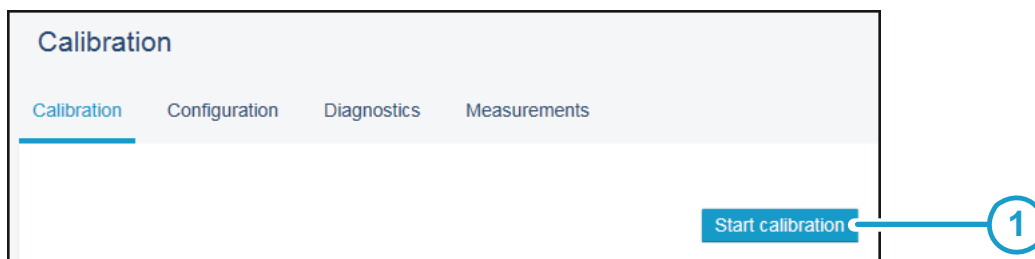


Figure 26 Start Calibration Button

1 **Start calibration** button on the **Calibration** tab

When you start the calibration mode, the **Start calibration** button is replaced with the **Stop calibration** button. The calibration mode remains active until you close it by selecting **Stop calibration**.

You can use other menus while the calibration mode is active, and return to the **Calibration** menu later to complete your adjustments.



Always close the calibration mode to return the probe and Indigo to normal operating mode. The measurement performance of the probe can be affected when used in calibration mode. You must close the calibration mode with the **Stop calibration** button also when no changes are made.

7.12.2 Restoring Factory Adjustment



Always restore factory adjustment before entering a new adjustment. This prevents any possible earlier adjustments having an effect on the new adjustment you make.

To restore factory adjustment:

1. Connect to the wireless configuration interface and open the **Calibration** menu.
2. Start the calibration mode with the **Start calibration** button.
3. On the **Calibration** tab, scroll down to the parameter you want to adjust (for example, **CO2 adjustment**) and select **Restore factory adjustment**.

CO2 adjustment

Reference value, point 1

Measured value, point 1

Reference value, point 2

Measured value, point 2

Store adjustment

Restore factory adjustment

4. Restore the factory adjustment with the **Restore factory adjustment** button for each parameter separately as needed.
5. To verify that the factory adjustment was restored, check the adjustment data information at the bottom of the **Calibration** tab view.
6. Close the calibration mode with the **Stop calibration** button.

7.12.3 Calibration PIN Code

General

Calibration PIN Code

Probe calibration can be locked and unlocked with a calibration PIN code in the Indigo transmitter's **Settings > Probe** menu. By default, the calibration PIN code is in place and calibration is enabled. Do not remove the PIN code from the probe settings unless you need to block access to calibration settings.

For GMP252, the calibration PIN code is **1300**.

7.12.4 1-point Adjustment with Indigo

Prepare the calibration reference (for example, a reference gas with a known concentration) before starting the adjustment.



When you enter a value into a field, the value is saved automatically when you exit the input field (for example, tap on an area outside of the field).

To make a 1-point adjustment with Indigo wireless configuration interface:

- ▶ 1. Connect to the wireless configuration interface and open the **Calibration** menu.
2. Start the calibration mode with the **Start calibration** button.



If you cannot enter configurations after selecting **Start calibration**, check that the calibration PIN code is in place in the **Settings > Probe** menu.

3. If you need to set environmental compensations, enable and set the required compensations on the **Configuration** tab.



Note that the environmental compensations you set on the **Configuration** tab and the compensations you set in the **Settings > Probe** menu are interconnected: the configuration set in either menu is applied to both.

4. Remove any possible previous adjustments by restoring the factory adjustment: select **Restore factory adjustment** for each parameter you are adjusting.

CO2 adjustment

Reference value, point 1

Measured value, point 1

Reference value, point 2

Measured value, point 2

5. Enter the calibration date and calibration information into the corresponding text fields.

Calibration information

Calibration date

Calibration text


6. Place the probe in the reference environment (adjustment point 1) and wait until the measurement has stabilized. You can follow the stabilization from the **Measurements** tab.
7. Enter the value of the reference (for example, **500** if calibrating with a 500 ppmCO₂ reference gas) into the **Reference value, point 1** field.
8. After you enter the reference value, the value of the **Measured value, point 1** field updates automatically.
9. After you have entered the reference point, select **Store adjustment** to save the adjustment.
10. Close the calibration mode with the **Stop calibration** button.
11. To check that the adjustment was carried out correctly, review the information in the **Adjustment data** fields at the bottom of the view.

7.12.5 2-point Adjustment with Indigo

To make a 2-point adjustment, you need a low reference and a high reference (select references that are near the low and high ends of your measurement range). Prepare the calibration references (for example, reference gases with known concentrations) before starting the adjustment.

To make a 2-point adjustment with Indigo wireless configuration interface:

- ▶ 1. Open the wireless configuration interface in the browser of your wireless device and open the **Calibration** menu.
- 2. Start the calibration mode with the **Start calibration** button.
- 3. If you need to set environmental compensations, enable and set the required compensations on the **Configuration** tab.
- 4. Remove any possible previous adjustments by restoring the factory adjustment: select **Restore factory adjustment** for each parameter you are adjusting.

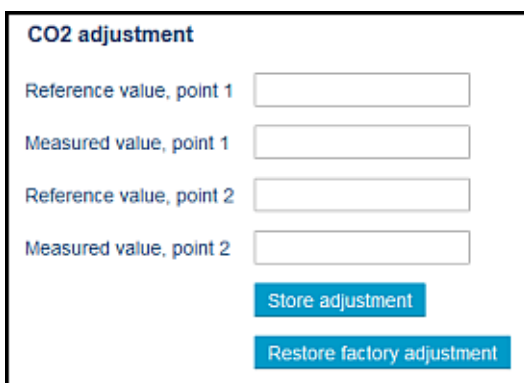

The screenshot shows a web interface titled "CO2 adjustment". It contains four input fields arranged in two pairs. The first pair is labeled "Reference value, point 1" and "Measured value, point 1". The second pair is labeled "Reference value, point 2" and "Measured value, point 2". Below these fields are two buttons: "Store adjustment" and "Restore factory adjustment".

5. Enter the calibration date and calibration information into the corresponding text fields.
6. Place the probe in the first reference environment (adjustment point 1) and wait until the measurement has stabilized.

7. Enter the value of the first reference (for example, **0** if calibrating with a 0 ppmCO₂ reference gas) into the **Reference value, point 1** field.
8. After you enter the reference value, the value of the **Measured value, point 1** field updates automatically.
9. Place the probe in the second reference environment (adjustment point 2) and wait until the measurement has stabilized.
10. Enter the value of the second reference (for example, **2000** if calibrating with a 2000 ppmCO₂ reference gas) into the **Reference value, point 2** field.
11. When both reference points have been entered, select **Store adjustment** to save the adjustment.
12. Close the calibration mode with the **Stop calibration** button.
13. To check that the adjustment was carried out correctly, review the information in the **Adjustment data** fields at the bottom of the view.

8. Operating with MI70 Indicator

8.1 Overview of MI70 Support

The probe is compatible with instruments that utilize the MI70 indicator, for example the GM70 Hand-Held Carbon Dioxide Meter. The MI70 indicator is a convenient service tool for viewing the measurement readings and performing calibration and one-point adjustment.



When MI70 is used with GMP252, it is recommended to use the rechargeable battery pack instead of alkaline batteries due to the relatively high power usage in CO₂ measurement.

8.1.1 Probe Warm-Up and MI70 Automatic Power Off

Note that the probe's warm-up time to full accuracy specification when starting up the probe can be several minutes. When you power the probe with the MI70 indicator, disable the automatic power off feature of MI70 to keep the probe powered on continuously in order to avoid probe restart. To ensure powering during measurements, it is recommended to use the MI70 charging adapter when possible.

8.2 Basic Display

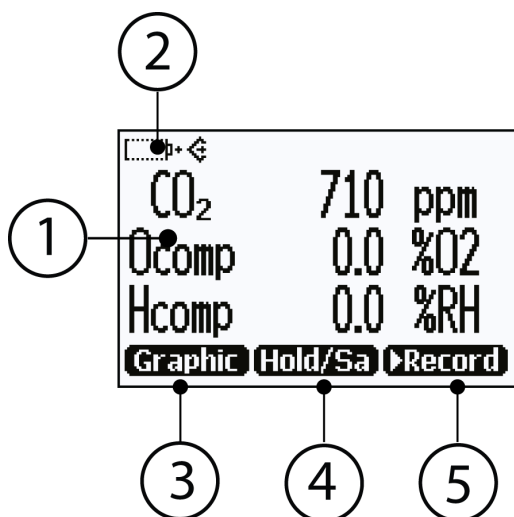


Figure 27 MI70 Basic Display

- 1 Measured parameter and compensations (up to three items on display simultaneously). You can change the shown items in **Main menu > Display > Quantities and units**.
- 2 Battery indicator. Shows current status (charge) of the battery.
- 3 Function key **Graphic** shows the readings as a curve.
- 4 Function key **Hold/Save** freezes the display and you can save the reading in the MI70 memory.
- 5 Function key **Record** is a quick access to the **Recording/Viewing** menu.

You can change the default function key shortcuts (**Graphic, Hold/Save, Record**) to other menus or functions in **Main menu > Settings > User interface > Program shortcut keys**.

8.3 Graphical Display

The graphical display shows you the measurements as a curve (the curve of the uppermost quantity shown in the basic display). From the curve you can examine the data trend and history of the last minutes.

To open the graphical display, select **Graphic** in the basic display or select **Main menu > Display > Graphic history > Show**.

To get the statistical info on the graph area (minimum, maximum, and average values), press **Info**.

To get the curve of the other selected quantities, press **Next**. To get the curves of all the quantities, press **Next** until the text **All** appears, and then select **All**.







To zoom in and out, press the up/down arrow keys.

To move back and forward in the timeline, use the left/right arrow keys.

8.4 Main Menu

In the main menu, you can configure the MI70 settings and basic display options, view information about the probe, access recordings and clear the memory, set alarms, start adjustments, and use the analog output option of the MI70 indicator.

To open the main menu and navigate in the menus:

- ▶ 1. Go to the basic display.
- 2. Press any arrow key, then select  **Open** (must be pressed within 5 seconds or the indicator returns to the basic display).
- 3. Move in the menus using the   buttons.
- 4. Select an item with the  button.
- 5. To return to the previous level, press .
- 6. To return to normal operation, press  **Exit**.

8.5 Connecting Probe to MI70 Indicator

- ▶ 1. If the probe is installed permanently into a device (for example, an incubator or a chamber), disconnect the probe from the connector.
- 2. If the MI70 indicator is on, turn it off.
- 3. Connect the probe to the MI70 indicator using the MI70 connection cable (Vaisala order code: CBL210472).

4. Turn on the MI70 indicator (time and date are requested at first startup). MI70 detects the probe and proceeds to show the measurement screen. The parameters measured by probe will start to show valid measurement results after a few seconds.

8.6 MI70 Indicator Parts

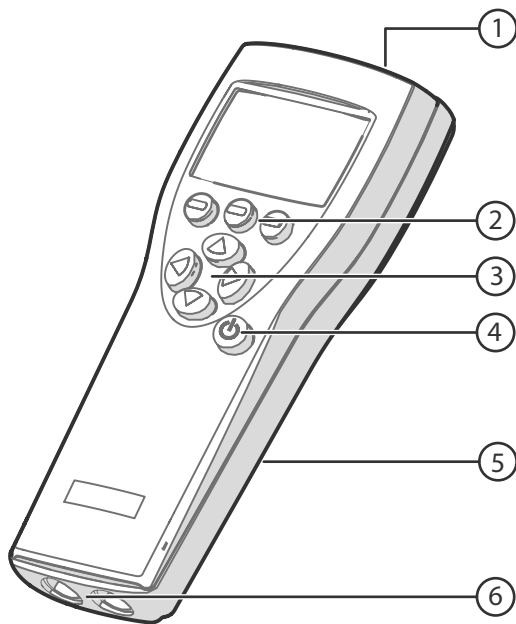







Figure 28 MI70 Indicator Parts

- 1 Charger socket
- 2 Function buttons . The functions change according to what you are doing with the indicator.
- 3 Arrow buttons:
 -  Move up in a menu
 -  Move down in a menu
 -  Enter a sub-menu
 -  Return to previous menu level
- 4 Power On/Off button
- 5 Battery compartment at the back of the indicator
- 6 Two ports (labeled I and II) for connecting probes and instruments.

To open menus, press an arrow button and then press the shortcut buttons. To activate a function shown above the shortcut button, press the shortcut button. To navigate in the menus, press arrow buttons.

8.7 Holding and Saving the Display

With the **Hold/Save** function, you can freeze a certain display reading. This reading can be saved in the MI70 memory and it will be available even after MI70 is disconnected from the transmitter.

1. In the basic display, select **Hold/Save**. Alternatively, select **Main menu > Display > Hold/Save display > Hold**.
2. Press **Save**.

- To view the saved display, go to basic display and select **Record > View recorded data**. Alternatively, select **Main menu > Recording/Viewing > View recorded data**.

A list of saved displays and data recordings appears. The icons on the left of the date and time indicate whether the file is a saved display or a longer recording of data:




Saved display



Data recording

- Select the saved display based on date and time by pressing the right arrow key.

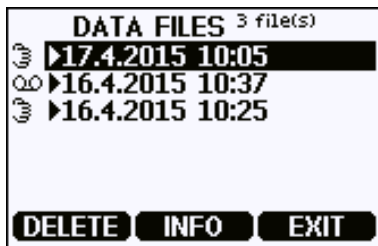


8.8 Recording Data

With MI70, you can record transmitter measurement data over a certain period at chosen intervals. These recordings are saved in MI70 memory and are available even after MI70 is disconnected from the transmitter.

8.9 Changing Environmental Compensation Settings with MI70 Indicator

You can see the compensation values that are currently used by the probe by selecting them as display quantities from **Main menu > Display > Quantities and Units**. The quantities are as follows:

- **Tcomp**: currently active temperature compensation value.
- **Pcomp**: currently active pressure compensation value.
- **Ocomp**: currently active oxygen concentration compensation value.
- **Hcomp**: currently active relative humidity compensation value.

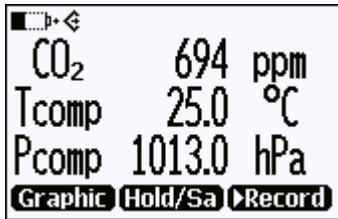Figure 29 CO₂ Reading with Tcomp and Pcomp on MI70 Screen

You can change the compensation settings from **Main menu > Settings > Measurement settings**.

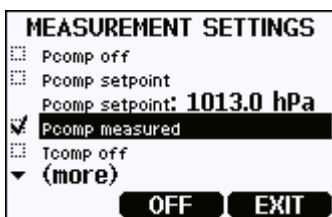


Figure 30 Probe Compensation Settings on MI70 Screen



When you turn a compensation off, the probe still shows a value for the corresponding display quantity (for example, Pcomp shows 1013.2 hPa). This is the default compensation value that is mathematically neutral for the probe's internal compensation model.



GMP252 cannot receive the compensation values from a second probe connected to MI70. Only direct configuration is supported.

8.10 Calibration and Adjustment with MI70 Indicator



Before using the MI70 indicator for calibration and adjustment, read the instructions in [Calibration and Adjustment \(page 94\)](#). Make sure that the environmental compensation settings of the probe are properly set for your calibration environment; see [Changing Environmental Compensation Settings with MI70 Indicator \(page 88\)](#).




When two probes are connected to the MI70 indicator, MI70 uses Roman numerals “I” and “II” to indicate which port the parameter or function in question is connected to.

8.10.1 1-Point Adjustment with an MI70-Compatible Reference Probe


- ▶ 1. Connect the GMP252 probe to Port I of the MI70 indicator.
2. Connect the calibrated reference probe to Port II. Make sure the reference probe is in the same environment as GMP252's sensor.
3. If you are using the calibration adapter to feed a calibration gas to GMP252, you must feed the same gas to the reference probe as well. Refer to the documentation of your reference probe on how to do this and what accessories you need.
4. Turn on the MI70 indicator.
5. Start the adjustment sequence from **Main menu > Functions > Adjustments**.



6. MI70 notifies you that automatic power off is disabled during adjustment mode, press **OK** to acknowledge.
7. To proceed with the adjustment, select the **CO2(I)** parameter in the **Select Quantity** screen. In the **Select Quantity** screen you can also view the currently used compensation values, and the **Last adjustment date** information. You can update the date and text using the **CDATE** and **CTEXT** commands on the serial line.
8. You may be prompted to check the environmental settings of the reference probe before proceeding. Press **Yes** to check the settings and **Exit** when you have checked and corrected the settings.
9. The adjustment mode is now active, and you can see the measured CO₂ readings and their difference on the screen. Allow the measurement to stabilize. To proceed with the adjustment, press **Adjust**.

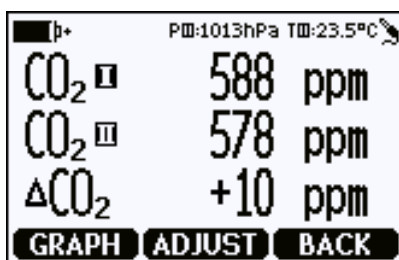


10. Select **To same as CO₂(II)**.

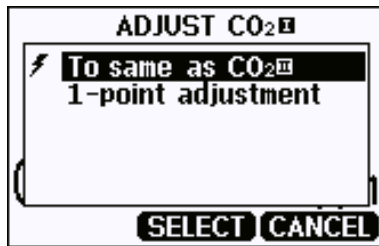

11. You will be prompted to confirm you want to adjust: select **Yes**.
12. If the adjustment is successful, MI70 will show the text **Adjustment Done**, after which you will return to the adjustment mode. At this point you can press **Back** and **Exit** to leave the adjustment mode. The adjustment is now completed. If the adjustment cannot be applied, MI70 will show the text **Cannot adjust**, possibly followed by a text stating the reason. A possible reason for an adjustment failure is attempting to apply a very large correction to the reading.


8.10.2 1-Point Adjustment with a Reference Gas

- ▶ 1. Connect GMP252 to Port I of the MI70 indicator.
2. Feed a calibration gas to the GMP252 using the calibration adapter accessory (Vaisala order code: DRW244827SP). If you are using ambient air as the calibration gas, you must have a reference meter in the same environment to verify the CO₂ concentration.
3. Turn on the MI70 indicator.
4. Start the adjustment sequence from **Main menu > Functions > Adjustments**.

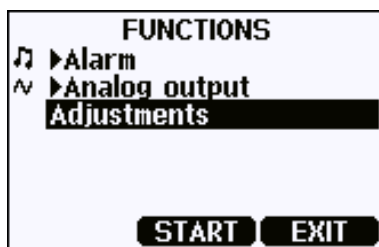


5. MI70 notifies you that automatic power off is disabled during adjustment mode, press **OK** to acknowledge.
6. Select the CO₂ parameter when prompted.
7. You may be prompted to check the environmental settings of the reference probe before proceeding. Press **Yes** to check the settings and **Exit** when you have checked and corrected the settings.


8. The adjustment mode is now active, and you can see the measured CO₂ reading on the screen. To proceed with the adjustment, press **Adjust**.

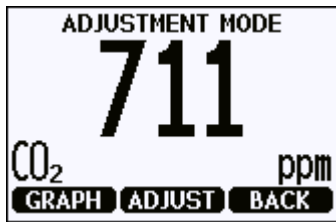

9. Select **1-point adjustment**.

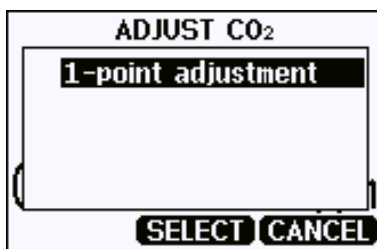

10. You will be prompted if you really want to adjust. Select **Yes**.
11. You are now in the 1-point adjustment screen. Allow the measurement to stabilize and press **Ready**.
12. Enter the CO₂ concentration of the reference gas and press **OK**.

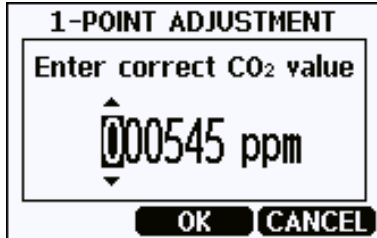

13. You will be prompted if you really want to adjust. Select **Yes**.
14. If the adjustment is successful, MI70 will show the text **Adjustment Done**, after which you will return to the adjustment mode. At this point you can press **Back** and **Exit** to leave the adjustment mode. The adjustment is now completed. If the adjustment cannot be applied, MI70 will show the text **Cannot adjust**, possibly followed by a text stating the reason. A possible reason for an adjustment failure is attempting to apply a very large correction to the reading.

9. Maintenance

9.1 Cleaning

You can clean the probe body by wiping it with a moist cloth. Standard cleaning agents can be used.

When cleaning, follow these precautions:

- Do not immerse the probe in liquid to clean it.
- Be careful not to block the filter when cleaning the probe. The optional sintered PTFE filter is especially sensitive to blockage.
- When changing the filter, you can use clean instrument air to gently blow any loose dirt and filter material from the sensor. Do not attempt to clean the optical surfaces in any other manner.

9.1.1 Chemical Tolerance

The following chemicals can be used to clean the probe:

- H₂O₂ (2000 ppm), non-condensing
- Alcohol-based cleaning agents such as ethanol and IPA (70 % Isopropyl Alcohol, 30 % water)
- Acetone
- Acetic acid



Avoid exposing the probe to chemicals for unnecessarily long periods of time. Do not immerse the probe in a chemical, and wipe chemicals off the probe after cleaning.

9.2 Changing the Filter

Change the filter to a new one if it shows visible signs of contamination or dirt. When changing the filter, use clean gloves to avoid blocking the pores of the new filter.

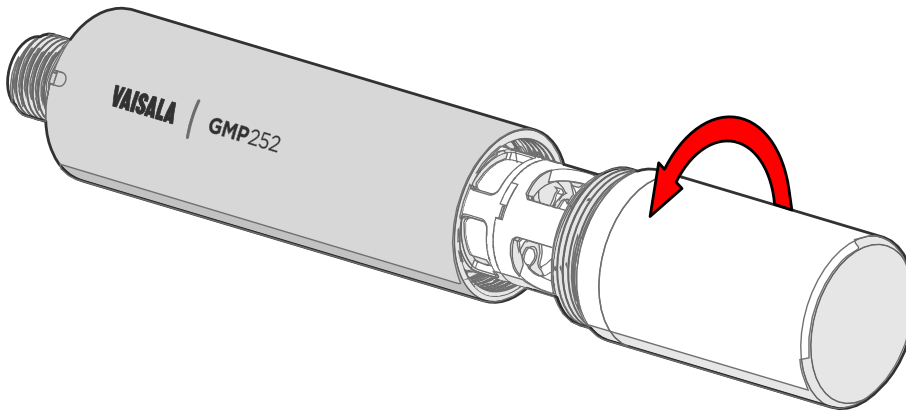


Figure 31 Opening the Filter



CAUTION! When changing the filter, you can use clean instrument air to gently blow any loose dirt and filter material from the sensor. Do not attempt to clean the optical surfaces in any other manner.

9.3 Calibration and Adjustment

Calibrate and adjust the CO₂ measurement of the probe as needed. Before starting, read through this section completely so that you are aware of your options, and the main factors that affect the result.



Performing an accurate calibration and adjustment takes some time and preparation. Instead of doing it yourself, you can also have a Vaisala Service Center calibrate and adjust your probe.



Calibration means comparing the measurement output of the device to a known reference, such as a known environment in a calibration chamber or the output of a reference instrument. Correcting the reading of the device so that it measures accurately is referred to as **adjustment**.

9.3.1 Calibration Setup

Using Hand-Held Meter as Reference

You can perform a 1-point calibration using a hand-held meter as a reference. You will need a calibrated reference instrument to compare against, for example a GM70 hand-held meter with a calibrated GMP222 probe.

With the probe and the reference instrument in the same space, allow the measurement to stabilize before comparing the readings. Try to provide as stable an environment as you can during this time. Avoid working around the probe and reference instrument during this time.

Using Calibration Gas as Reference

There are two easy ways to use a calibration gas as a reference:

- You can supply the gas to the probe using the calibration adapter accessory (Vaisala order code DRW244827SP). Gas flow should be in the range 0.5 ... 1.1 l/min, recommendation is 1 l/min. Allow the measurement to stabilize for three minutes before starting the calibration.
- You can fill the entire incubator with the calibration gas. You can use calibration gas as a reference by putting the probe in a suitable chamber (for example, an incubator) and filling that chamber with the calibration gas.

To perform a two-point adjustment, you need two calibration gases: one gas that is below 1000 ppmCO₂ (low-end reference) and one that is above 2000 ppmCO₂ (high-end reference).

When supplying the gas from a gas bottle, make sure the gas bottle has stabilized to room temperature before starting.

9.3.2 Effect of Environmental Compensations

The probe has various environmental compensations that improve its CO₂ measurement accuracy (see [Environmental Compensation \(page 15\)](#)). As the calibration and adjustment environment may differ from the actual measurement environment, you must make sure that the compensation settings are properly set. Here are some key points to remember:

- Pressure and temperature compensations have a significant effect on accuracy. If you are using setpoint values instead of the values from the built-in temperature sensor or an integrated system, make sure to correct the setpoints so that they correspond to your calibration situation. Consider switching temperature compensation to use the internal sensor and/or integrated system when calibrating, and then switching back when calibration and adjustment is done.
- The effect of background gas compensations for humidity and oxygen may be significant when using calibration gases, since these gases are often dry and oxygen-free. For example, pure nitrogen gas is typically used as a convenient 0 ppm CO₂ reference. As it does not contain any oxygen or humidity, the compensations for them must be set to zero.
- Remember to restore the normal compensation settings after completing calibration and adjustment. If you are integrating the calibration functionality of the probe as part of a control software, also implement proper handling of the environmental compensations.

More Information

- [Environmental Compensation \(page 15\)](#)

9.3.3 Limits of Adjustment

The probe limits the amount of adjustment that is allowed to the CO₂ measurement. The maximum correction that you can apply is 1000 ppm + 25 % of the probe's uncorrected reading. Previous user adjustments do not affect this limit (the correction is not cumulative). This feature limits the possible error introduced by incorrect adjustment.

For example, if you are adjusting using a 5000 ppmCO₂ calibration gas, the maximum correction you can apply is approximately 2250 ppm. Attempting to apply a greater adjustment will fail. Notification of failure from the probe depends on the interface you are using for adjustment.

9.3.4 Adjustment Types

You can adjust the CO₂ measurement of the probe in one or two points.

- One-point adjustment is recommended if you are interested in maintaining a fixed CO₂ level. For best result, use a calibration gas with a CO₂ concentration that is close to the intended level.
- Two-point adjustment is recommended if you typically measure a variable CO₂ level.

Available adjustment functions depend on the interface you use to operate the probe. If you want to integrate the functionality into a control system, the Modbus interface and the Vaisala industrial protocol are recommended. If you want to compare the reading of the probe to a reference instrument and adjust it accordingly, use an MI70 hand-held indicator and a reference probe.

Vaisala Industrial Protocol

Vaisala industrial protocol supports 1-point and 2-point adjustment with the **cco2** command. Configuration of the environmental compensation settings can be done using serial line commands.

Modbus

The environmental compensation settings can be configured using Modbus registers.

MI70 Hand-Held Indicator

The MI70 hand-held indicator supports 1-point adjustment, either using a calibration gas or using a reference instrument that is connected to the MI70.

Vaisala Insight PC software

You can carry out 1-point and 2-point adjustments and change the environmental compensation settings with the Insight software (requires USB cable 242659).

Vaisala Indigo transmitters

You can use the Indigo transmitter's wireless configuration interface to carry out 1-point and 2-point adjustments and change the environmental compensation settings.

More Information

- [Calibration and Adjustment \(page 49\)](#)
- [Configuration Registers \(page 114\)](#)
- [Calibration and Adjustment with MI70 Indicator \(page 89\)](#)
- [Indigo Calibration Overview \(page 78\)](#)

9.3.5 DRW244827SP Calibration Adapter

The optional calibration adapter accessory can be used to feed a reference gas to the probe through a gas port when calibrating. Gas flow should be in the range 0.5 ... 1.1 l/min, recommendation is 1 l/min. Allow the measurement to stabilize for three minutes before starting the calibration.

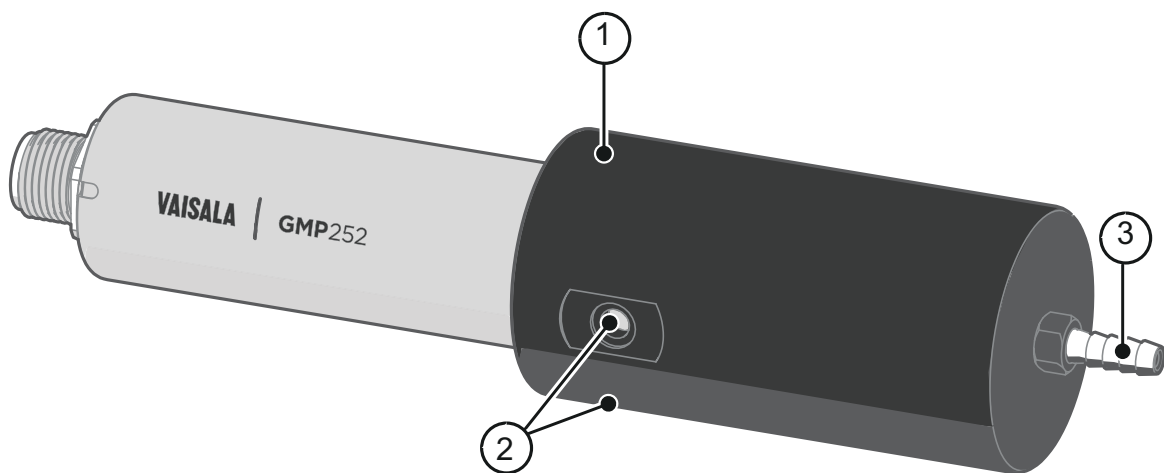


Figure 32 DRW244827SP Calibration Adapter with Probe Inserted

- 1 O-ring inside the adapter
- 2 Gas outlet on each side of the adapter
- 3 Gas port (port outer diameter 4.6 mm, port hole inner diameter 2 mm, suitable for tubing with 4 mm inner diameter)

10. Troubleshooting

10.1 Problem Situations

Problem	Possible Cause	Remedy
Analog output reading is unchanging and appears incorrect.	Analog output is in error state.	Remove the cause of the error state and the analog output will recover its normal function.
Probe outputs stars "*****" on serial line instead of measurement data.	Incorrect supply voltage.	Check the power supply. Check the active errors using the ERRS command on the serial line.
	Unsuitable operating environment.	Verify that the operating environment is within specified operating limits.
Unable to access probe on the RS-485 line.	Incorrect wiring.	Check that the RS-485 connection is wired correctly.
	Probe in POLL mode with unknown address.	Power cycle or reset the probe and try again.
CO ₂ measurement not working.	Condensation on the sensor.	Remove the filter and check if condensation has formed on the sensor. If yes, dry out the condensation with instrument air and insert a new dry filter. Keep the probe powered and operating to prevent re-occurrence.

More Information

- [Wiring \(page 25\)](#)
- [Analog Output Error State \(page 100\)](#)

10.2 Error Messages

The error messages are categorized according to the severity of the status:

- **Critical errors** are fatal to the operation of the unit. It may not be able to respond to communication at all, and will not measure correctly.
- **Errors** prevent CO₂ measurement and cause the analog outputs to be set to the error state. Depending on the problem, errors may resolve themselves. For example, sensor heating will eventually dry out condensation on the optical surfaces.
- **Warnings** do not prevent normal operation but may indicate possible problems.
- **Status** indicates a known state of the unit.

Error Message	Description	Recommended Action
Critical errors		
Program memory crc critical error	Program memory is corrupted.	Fatal error, contact Vaisala.
Parameter memory crc critical error	Parameter memory is corrupted.	Fatal error, contact Vaisala.
Errors		
Low supply voltage error		Check supply voltage.
Internal 30 V error	Low internal 30 V voltage.	
Low RX signal error	Low input signal. Can be caused by dirt or condensation on the optical surfaces.	Wait to see if condensation is removed by heat.
Internal 8 V error	Low internal 8 V voltage.	
RX signal cut error	Signal distortion (EMC interference)	
Out of measurement range error	CO ₂ concentration is too high to measure.	Wait for CO ₂ concentration to fall into the measurable range.
Sensor heater error	Sensor heater resistance is out of range.	
IR temperature error	IR source temperature error.	
FPI slope error	Signal receiver error.	Contact Vaisala.
Internal 2.5 V error	Internal 2.5 V voltage out of range.	
Internal 1.7 V error	Internal 1.7 V voltage out of range.	
Low IR current error	IR source failure.	Contact Vaisala.
Warnings		
Signal too low warning	Low input signal. Can be caused by dirt or condensation on the optical surfaces.	Continue normally.
Cut warning	EMC interference error limit approaching.	Check for EMC interference sources.
Unexpected restart detected	Transmitter is reset by watchdog process.	Continue normally.
Status messages		
CO ₂ adjustment mode active		Complete the CO ₂ adjustment.

10.3 Analog Output Error State

The probe sets the analog output channel into a defined error level instead of the measured result in two situations:

- Probe detects a measurement malfunction. This means an actual measurement problem, such as sensor damage or unsuitable environmental conditions.
- Measured value(s) are significantly outside the scaled output range.

The default error level depends on the output type:

Output	Default Error Level
0 ... 20 mA	23 mA
4 ... 20 mA	2 mA
0 ... 5 V	0 V
0 ... 10 V	0 V

The probe resumes normal operation of the analog output when the cause of the error state is removed.

More Information

- [Analog Output Overrange Behavior \(page 18\)](#)

10.4 Indigo Wireless Connection Troubleshooting

The following table contains troubleshooting information related to accessing the wireless (WLAN) configuration interface of Vaisala Indigo transmitters.

Problem	Possible Cause	Remedy
The wireless device has connected to the Indigo access point, but the configuration interface does not launch.	The device you are using to connect to Indigo does not launch the browser automatically after connecting to the access point.	After connecting to Indigo, open your browser application.
	The wireless connection requires an authentication or acknowledgement before the Indigo interface opens in your browser.	Check your device's notifications to see if an authentication or login prompt is present for the Indigo connection. Acknowledge the connection and open your browser application if the interface does not launch automatically.
The Indigo access point does not show up in your device's list of available WLAN connections.	Indigo access point is not enabled or an error has occurred.	Switch off the Indigo WLAN connection, enable the connection again and retry.
	Your device is too far from the transmitter or obstacles are blocking the signal.	Move closer to the transmitter and refresh your device's access point list.
Indigo shows up in the list of available wireless connections, but connecting to it does not work.	A device is already connected to the Indigo access point.	Ensure that your device is the only one that is connecting to the wireless configuration interface.

Problem	Possible Cause	Remedy
The interface does not open in the browser.	The browser has issues with loading the landing page.	Enter the default Indigo IP address http://192.168.1.1 in the browser's address bar.
Cannot connect to the Indigo access point with iPhone.	The iPhone WLAN settings prevent establishing a connection.	See the iPhone connection instructions in the Indigo transmitter's <i>User Guide</i> .
Indigo does not respond when pressing the wireless connection activation button.	WLAN functionality has been disabled with the WLAN ON/OFF DIP switch on Indigo's circuit board.	Enable WLAN functionality with the WLAN ON/OFF DIP switch. See the instructions in the Indigo transmitter's <i>User Guide</i> .

11. Technical Data

11.1 GMP252 Specifications

Table 47 Measurement Performance

Property	Description/Value
Measurement range	0 ... 10 000 ppmCO ₂ (up to 30 000 ppmCO ₂ with reduced accuracy)
Accuracy at 25 °C and 1013 hPa (incl. Repeatability and Non-Linearity)	
0 ... 3000 ppmCO ₂	±40 ppmCO ₂
3000 ... 10 000 ppmCO ₂	±2 % of reading
Up to 30 000 ppmCO ₂	±3.5 % of reading
Calibration Uncertainty	
at 2000 ppmCO ₂	±38 ppmCO ₂
at 10 000 ppmCO ₂	±105 ppmCO ₂
Long-Term Stability	
0 ... 3000 ppmCO ₂	±60 ppmCO ₂ /year
3000 ... 6000 ppmCO ₂	±150 ppmCO ₂ /year
6000 ... 10 000 ppmCO ₂	±300 ppmCO ₂ /year
Temperature Dependence 0 ... 10 000 ppmCO₂	
with compensation, -10 ... +50 °C	±0.05 % of reading/°C
with compensation, -40 ... +60 °C	< ±0.1 % of reading/°C
without temperature compensation at 2000 ppmCO ₂ (typical)	-0.5 % of reading/°C
Pressure Dependence	
with compensation at 0 ... 10 000 ppmCO ₂ , 500 ... 1100 hPa	±0.015 % of reading/hPa
without compensation (typical)	+0.15 % of reading/hPa
Humidity Dependence	
with compensation, 0 ... 10 000 ppmCO ₂ , 0 ... 100 %RH	±0.7 % of reading (at +25 °C (+77 °F))
without compensation (typical)	+0.05 % of reading/%RH
O₂ Dependence	

Property	Description/Value
with compensation, 0 ... 10 000 ppm%CO ₂ , 0 ... 90 %O ₂	±0.6 % of reading (at +25 °C (+77 °F))
without compensation (typical)	-0.08 % of reading/%O ₂
Start-Up, Warm-Up and Response Time	
Start-up time at +25 °C	< 12 s
Warm-up time for full spec.	< 2 min
Response time (T90) with standard filter	< 1 min
Response time (T90) with spray shield	< 3 min
Flow-Through Option	
Response time (T90) with > 0.1 l/min	30 s
Flow rate dependence < 1 l/min flow	no effect
Flow rate dependence 1 ... 10 l/min flow	< 0.6% of reading l/min
Gas flow operating range	< 10 l/min
Gas flow recommended range	0.1 ... 0.8 l/min

Table 48 Operating Environment

Property	Description/Value
Operating temperature of CO ₂ measurement	-40 ... +60 °C (-40 ... +140 °F)
Storage temperature	-40 ... +70 °C (-40 ... +158 °F)
Humidity	0 ... 100 %RH, non-condensing
Condensation prevention	Sensor head heating when power on
EMC compliance	EN61326-1, Generic Environment
Chemical tolerance (temporary exposure during cleaning)	<ul style="list-style-type: none"> • H₂O₂ (2000 ppm, non-condensing) • Alcohol-based cleaning agents (for example ethanol and IPA) • Acetone • Acetic acid
Pressure	
Compensated	500 ... 1100 hPa
Operating	< 1.5 bar

Table 49 Mechanical Specifications

Property	Description/Value
Weight, probe	58 g (2.05 oz)

Property	Description/Value
Connector type	M12 5-pin male
IP rating, probe body	IP65
Materials	
Probe housing material	PBT plastic
Filter	PTFE
Connector	Nickel plated brass
Dimensions	
Probe diameter	25 mm (0.98 in)
Probe length	130 mm (5.12 in)

Table 50 Inputs and Outputs

Property	Description/Value
Digital output	Over RS-485: <ul style="list-style-type: none"> • Modbus • Vaisala Industrial Protocol
Analog output	<ul style="list-style-type: none"> • 0 ... 5/10 V (scalable), min load 10 kΩ • 0/4 ... 20 mA (scalable), max load 500 Ω
Operating voltage	
With digital output in use	12 ... 30 VDC
With voltage output in use	12 ... 30 VDC
With current output in use	20 ... 30 VDC
Power consumption	
Typical (continuous operation)	0.4 W
Maximum	0.5 W
When connected to Indigo 200 transmitter	
Analog output	3 voltage (V) or current (mA) outputs: <ul style="list-style-type: none"> • 0 ... 10 VDC / 0 ... 5 VDC / 0 ... 1 VDC / 1 ... 5 VDC (min load 1kΩ) • 0 ... 20 mA / 4 ... 20 mA (max load 500 Ω)
Relays	2 configurable relays
Power supply input	Nominal 24 V, range: <ul style="list-style-type: none"> • 15 ... 40 VDC • 20 ... 28 VAC
Power consumption	Max. 3.5 W (transmitter + probe total max. consumption)

11.2 Spare Parts and Accessories



Information on spare parts, accessories, and calibration products is available online at www.vaisala.com and store.vaisala.com.

Name	Order Code
Porous sintered PTFE filter for GMP252	DRW244221SP
Probe cable with open wires (1.5 m (4.9 ft))	223263SP
Probe cable with open wires and 90° plug (0.6 m (1.97 ft))	244669SP
Probe cable with open wires (10 m (32.8 ft))	216546SP
Flow-through adapter with gas ports	ASM212011SP
USB cable for PC connection ¹⁾	242659
MI70 connection cable for probe	CBL210472
Flat cable for GMP250 probes, M12 5-pin	CBL210493SP
Probe mounting clips (2 pcs)	243257SP
Probe mounting flange	243261SP
Calibration adapter	DRW244827SP
Spray shield	ASM212017SP
Radiation shield DTR250	DTR250
Radiation shield DTR250 with pole mounting kit	DTR250A

¹⁾ Vaisala Insight software for Windows® available at www.vaisala.com/insight.

11.3 GMP252 Probe Dimensions

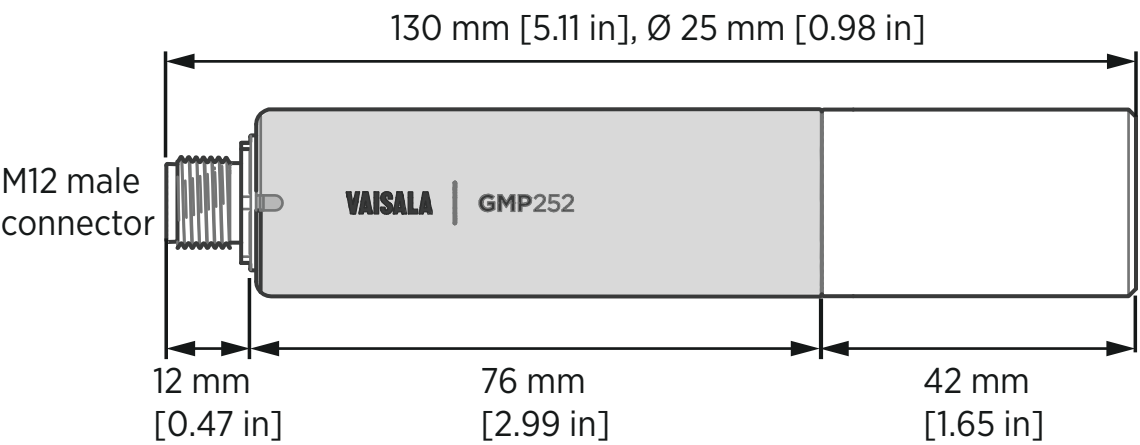


Figure 33 GMP252 Dimensions

11.4 243261SP Mounting Flange Dimensions

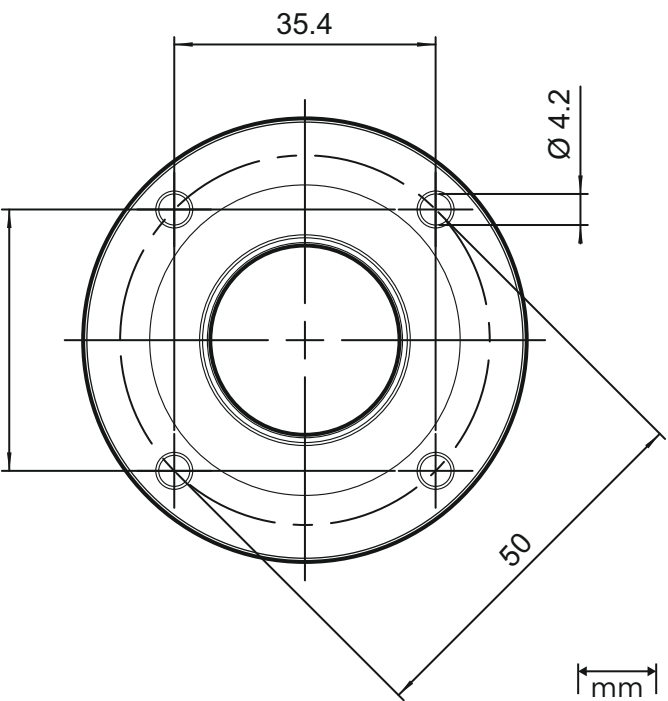


Figure 34 243261SP Mounting Flange Dimensions

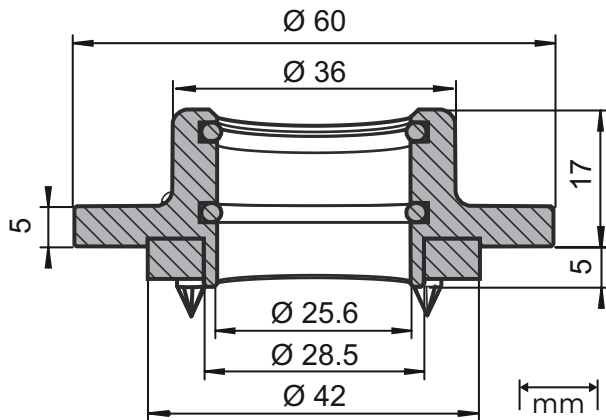


Figure 35 243261SP Mounting Flange Dimensions, Cross Section

11.5 DRW244827SP Calibration Adapter Dimensions

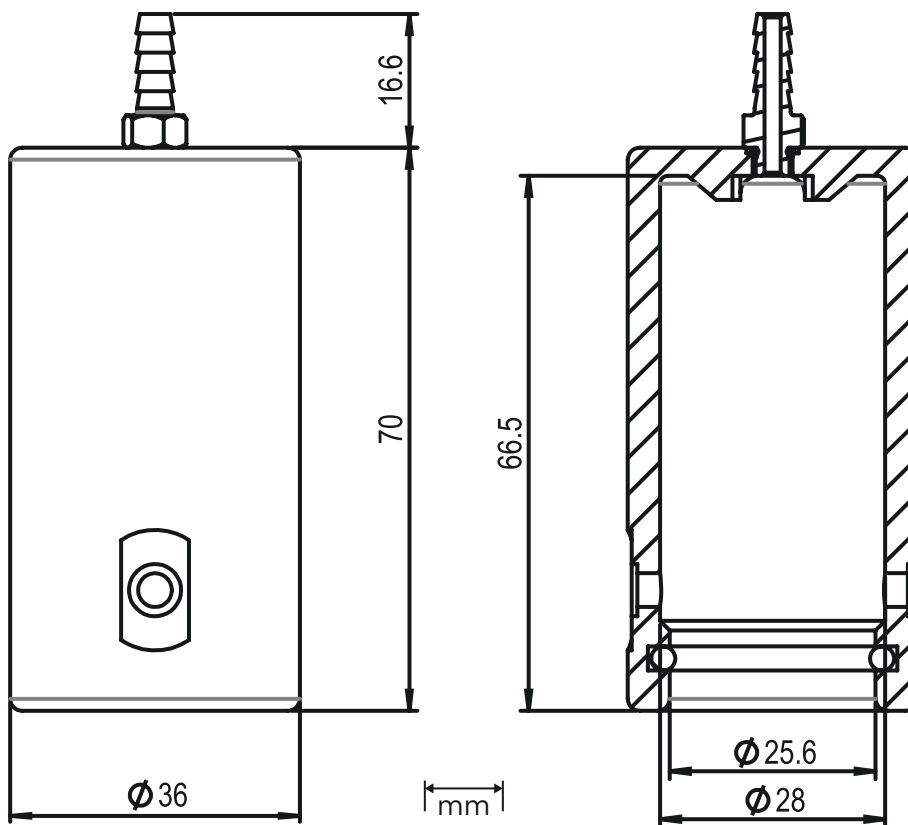


Figure 36 DRW244827SP Calibration Adapter Dimensions

11.6 ASM212017SP Spray Shield Dimensions

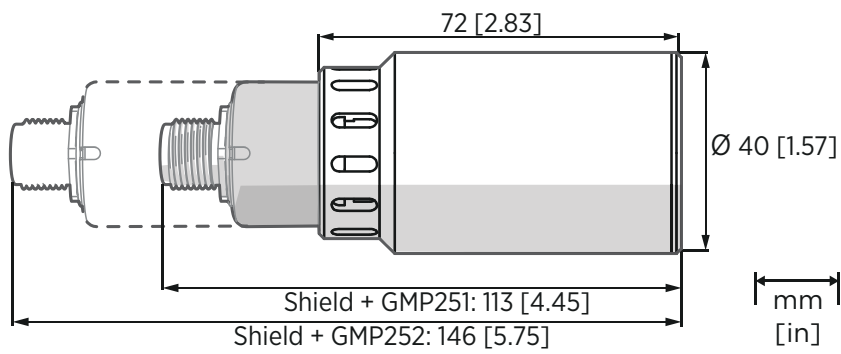


Figure 37 ASM212017SP Spray Shield Dimensions

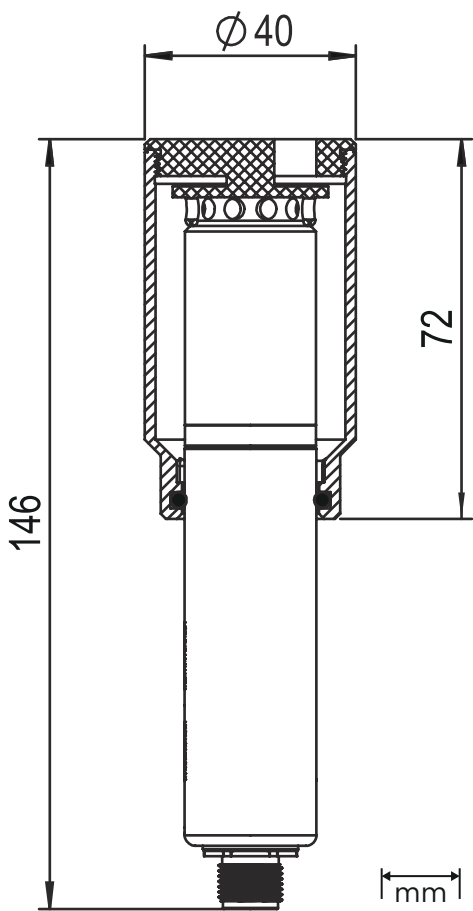


Figure 38 GMP252 Spray Shield Cross Section

11.7 DTR250 Radiation Shield Dimensions

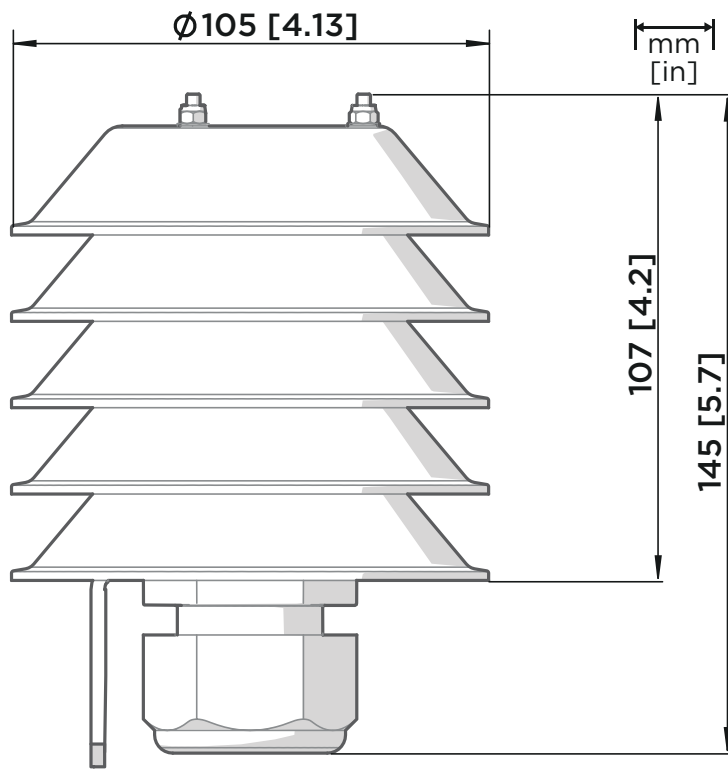


Figure 39 DTR250 Radiation Shield Dimensions (mm)

11.8 DTR250A Pole Mounting Kit Dimensions

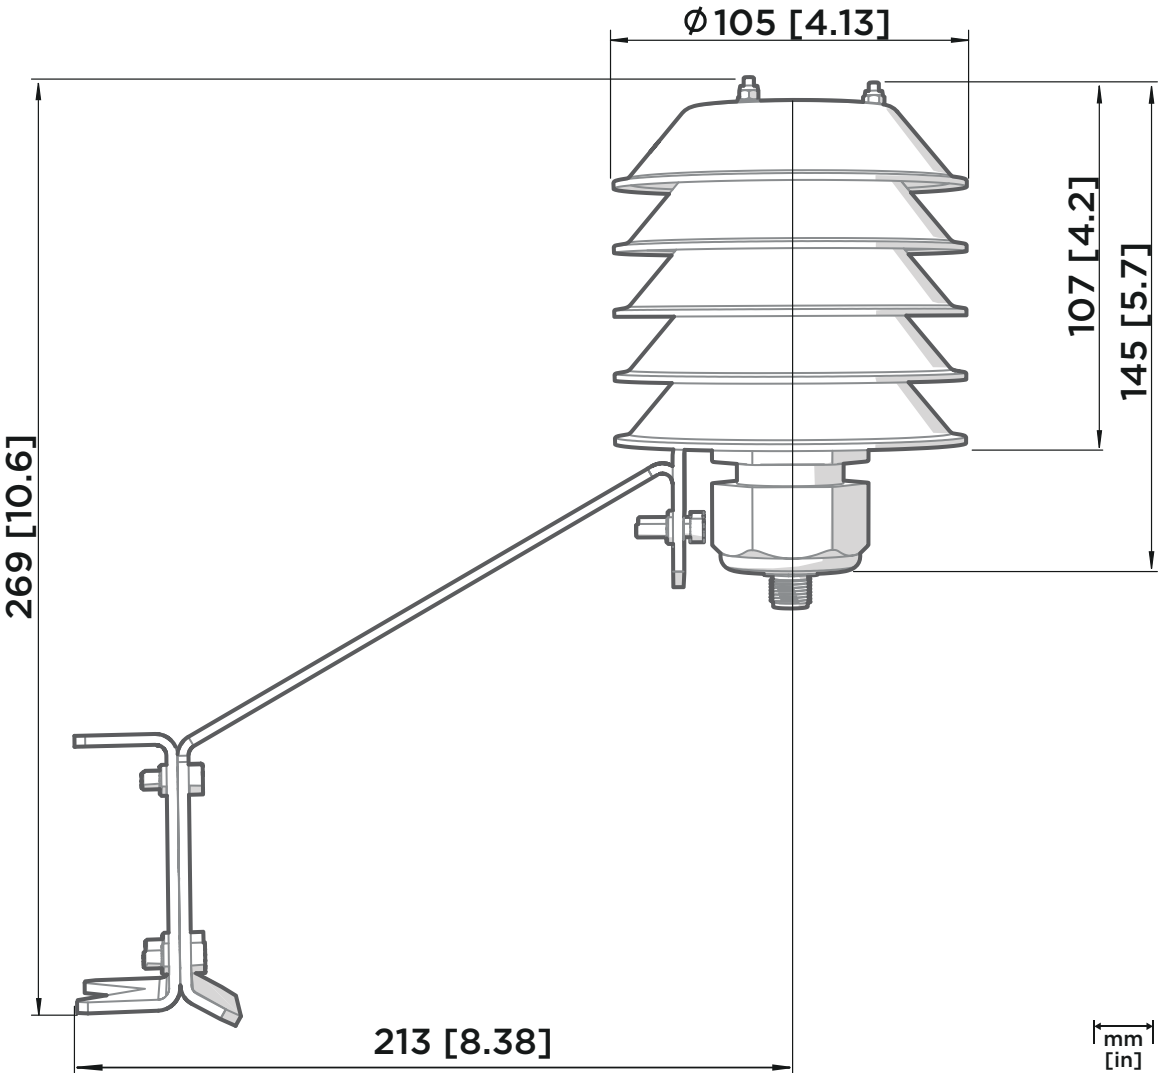


Figure 40 DTR250A Pole Mounting Kit Dimensions (in mm [inch])

Appendix A. Modbus Reference

A.1 Function Codes

Table 51 Supported Function Codes

Function Code (Decimal)	Function Code (Hexadecimal)	Name
03	03 _{hex}	Read Holding Registers
16	10 _{hex}	Write Multiple Registers
43/14	2B _{hex} / 0E _{hex}	Read Device Identification

A.2 Modbus Registers



CAUTION! Registers are numbered in decimal, starting from one. Register addresses in actual Modbus messages (Modbus Protocol Data Unit (PDU)) are in hexadecimal and start from zero. Subtract 1 from the register number presented in this manual to get the address used in the Modbus message. For example, the register number 769 (Modbus address) corresponds to address 0300_{hex} in the Modbus message.

Accessing unavailable (temporarily missing) measurement data does not generate an exception. “Unavailable” value (a quiet NaN for floating point data or 0000_{hex} for integer data) is returned instead. An exception is generated only for any access outside the applicable register ranges.

A.2.1 Measurement Data

Table 52 Modbus Measurement Data Registers (Read-Only)

Register Number (Decimal)	Address (Hexadecimal)	Register Description	Data Format	Unit
1	0000 _{hex}	Measured CO ₂ value	32-bit float	ppm
3	0002 _{hex}	Compensation T	32-bit float	°C
5	0004 _{hex}	Measured T	32-bit float	°C
257	0100 _{hex}	Measured CO ₂ value	16-bit signed integer	ppm (up to 32 000 ppm)

Register Number (Decimal)	Address (Hexadecimal)	Register Description	Data Format	Unit
258	0101 _{hex}	Measured CO ₂ value	16-bit signed integer	ppm ¹⁾ (scaled, up to approx. 320 000 ppm)

1) The ppm output of the second Measured CO₂ value register (number 258) is scaled and must be multiplied by 10.

A.2.2 Configuration Registers



CAUTION! Default power-up values (registers 513-519) are written into non-volatile EEPROM memory. The EEPROM memory implementation has a limit of 30000 writes, and is intended to be used only when saving long-term or permanent configurations. Use the volatile memory (registers 521 ... 527, values cleared on power-up) for non-permanent configurations (for example, if the probe is used in a system that regularly updates the compensation values).

Table 53 Modbus Configuration Data Registers (Writable)

Register Number (Decimal)	Address (Hexadecimal)	Register Description	Data Format	Unit / Valid Range
513	0200 _{hex}	Power-up value for pressure compensation	32-bit float	hPa 700 ... 1500 hPa Operating <1.5 bar (Init/default: 1013.25)
515	0202 _{hex}	Power-up value for temperature compensation	32-bit float	°C -40 ... +80 (Init/default: 25)
517	0204 _{hex}	Power-up value for humidity compensation	32-bit float	%RH 0 ... 100 % (Init/default: 0)
519	0206 _{hex}	Power-up value for oxygen compensation	32-bit float	%O ₂ 0 ... 100 % (Init/default: 0)
521	0208 _{hex}	Volatile (value cleared at probe reset) pressure compensation	32-bit float	Range 700 ... 1500 hPa (Init copied from power-up value)
523	020A _{hex}	Volatile (value cleared at probe reset) temperature compensation	32-bit float	Range -40 ... +80 °C (Init copied from power-up value)

Register Number (Decimal)	Address (Hexadecimal)	Register Description	Data Format	Unit / Valid Range
525	020C _{hex}	Volatile (value cleared at probe reset) humidity compensation	32-bit float	Range 0 ... 100 %RH (Init copied from power-up value)
527	020E _{hex}	Volatile (value cleared at probe reset) oxygen compensation	32-bit float	Range 0 ... 100 %O ₂ (Init copied from power-up value)
769	0300 _{hex}	Modbus address	16-bit integer	Valid range 1 ... 247 (default: 240)
770	0301 _{hex}	Serial speed	enum	Valid range 4800 ... 115200 0 = 4800 1 = 9600 2 = 19200 3 = 38400 4 = 57600 5 = 115200 (default: 2 (19200))
771	0302 _{hex}	Serial parity	enum	0 = None 1 = Even 2 = Odd (default: 0 (None))
772	0303 _{hex}	Serial stop bits	16-bit integer	Valid range 1...2 (default: 2)
773	0304 _{hex}	Pressure compensation mode	enum	0 = Off 1 = On (default: 1 (On))
774	0305 _{hex}	Temperature compensation mode	enum	0 = Off 1 = Given 2 = Measured (default: 2 (Measured))
775	0306 _{hex}	Humidity compensation mode	enum	0 = Off 1 = On (default: 0 (Off))
776	0307 _{hex}	Oxygen compensation mode	enum	0 = Off 1 = On (default: 0 (Off))

Register Number (Decimal)	Address (Hexadecimal)	Register Description	Data Format	Unit / Valid Range
777	0308 _{hex}	CO ₂ filtering factor	16-bit integer	Valid range 0 ... 100 (default: 100 (no filtering)). For information on setting the filtering factor, see Filtering Factor (page 120) .



To apply an accurate relative humidity compensation (775), you must also enable temperature compensation (774) and pressure compensation (773).

A.2.3 Status Registers

Table 54 Modbus Status Registers (Read-Only)

Register Number (Decimal)	Address (Hexadecimal)	Register Description	Data Format	Notes
2049	0800 _{hex}	Device status	16-bit	0 = Status OK. 1 = Critical error. 2 = Error. 4 = Warning.
2050	0801 _{hex}	CO ₂ status	16-bit	0 = Status OK. 2 = CO ₂ reading not reliable. Appears during transmitter start-up. 256 = Measurement not ready. Appears during transmitter start-up.



Multiple statuses can be present simultaneously. In those cases, the value of the status register is the sum of the status values. For example, the value of the device status register is **6** if a warning (**4**) and an error (**2**) are present simultaneously.

More Information

- [Error Messages \(page 99\)](#)

A.2.4 Device Identification Objects

Table 55 Device Identification Objects

Object ID (Decimal)	Object ID (Hexadecimal)	Object Name	Example Contents
0	00 _{hex}	VendorName	"Vaisala"
1	01 _{hex}	ProductCode	"GMP25x Carbon Dioxide Probe "
2	02 _{hex}	MajorMinorVersion	Software version (for example "1.2.3")
3	03 _{hex}	VendorUrl	"http://www.vaisala.com/"
4	04 _{hex}	ProductName	"GMP25X "
128	80 _{hex}	SerialNumber ¹⁾	Transmitter serial number (for example, "K0710040")
129	81 _{hex}	Calibration date ¹⁾	Date of the factory calibration
130	82 _{hex}	Calibration text ¹⁾	Information text of the factory calibration

1) Vaisala-specific device information object

A.3 Modbus Communication Examples

Reading CO₂ Value




Device address used in the following examples is 240 (F0_{hex}).

The values returned by the device differ depending on the ambient conditions and/or device settings. Your device might not return exactly same values.

Request		Response	
Bytes on the Line (Hexadecimal)	Description	Bytes on the Line (Hexadecimal)	Description
(silence for 3.5 bytes)	Start of Modbus RTU frame	(silence for 3.5 bytes)	Start of Modbus RTU frame
F0 _{hex}	GMP25x address	F0 _{hex}	GMP25x address
03 _{hex}	Function (Read Holding Registers)	03 _{hex}	Function (Read Holding Registers)
00 _{hex}	Register address	04 _{hex}	Number of data bytes
00 _{hex}		D4 _{hex}	Value of first register (least significant word)
00 _{hex}	Number of 16-bit registers to read (2)	7A _{hex}	
02 _{hex}		43 _{hex}	Value of second register (most significant word)
D1 _{hex}	Modbus RTU checksum	E8 _{hex}	
2A _{hex}		33 _{hex}	Modbus RTU checksum
(silence for 3.5 bytes)	End of Modbus RTU frame	AB _{hex}	
		(silence for 3.5 bytes)	End of Modbus RTU frame

Communication Description	
Register address	1 (1-based Modbus documentation format) = 0000 _{hex} (0-based format used in actual communication).
Data format	Two 16-bit Modbus registers interpreted as IEEE 754 binary32 floating point value, least significant word first.
Returned value	43E8D47Ah, which is binary32 representation of 465.65997 (ppm).

Writing Volatile Compensation Pressure Value

Request		Response		
Bytes on the Line (Hexadecimal)	Description	Bytes on the Line (Hexadecimal)	Description	
(silence for 3.5 bytes)	Start of Modbus RTU frame	(silence for 3.5 bytes)	Start of Modbus RTU frame	
F0 _{hex}	GMP25x address	F0 _{hex}	GMP25x address	
10 _{hex}	Function (Write Multiple Registers)	10 _{hex}	Function (Write Multiple Registers)	
02 _{hex}	Register address	02 _{hex}	Register address	
08 _{hex}		08 _{hex}		
00 _{hex}	Number of registers to write (2)	00 _{hex}	Number of 16-bit registers written (2)	
02 _{hex}		02 _{hex}		
04 _{hex}	Number of data bytes	D4 _{hex}	Modbus RTU checksum	
50 _{hex}	Value for the first register (least significant word)	93 _{hex}		
00 _{hex}		(silence for 3.5 bytes)	End of Modbus RTU frame	
44 _{hex}	Value for the second register (most significant word)	<div><p>The response to a write function informs that the function was correctly received by the device. It does not guarantee that the written value was accepted by the device (for example, in case of out-of-range values). To verify that the value was really accepted by the device, read the register value after writing.</p></div>		
7D _{hex}				
0E _{hex}	Modbus RTU checksum			
B7 _{hex}				
(silence for 3.5 bytes)	End of Modbus RTU frame			

Communication Description	
Register address	521 (1-based Modbus documentation format) = 0208 _{hex} (0-based format used in actual communication).
Data format	Two 16-bit Modbus registers interpreted as IEEE 754 binary32 floating point value, least significant word first.
Value to write	1013.25 (hPa), in binary32 format 447D5000 _{hex} .

A.4 Filtering Factor

Modbus register 777 sets the CO₂ filtering factor.

The filtering factor affects the speed at which the latest CO₂ measurement is integrated into the output of the probe. A new measurement is produced approximately every two seconds.

By default, the filtering factor is set to 1.0, which means the latest measurement is shown directly in the output, without any filtering. If the measuring environment produces occasional exceptionally high or low readings that need to be averaged out in the output, filtering can be applied.

To apply filtering, you need to set a filtering factor that determines how much the previous measurements affect the calculation of measurement output. For example, when using filtering factor of 0.1, the new output is a combination of previous measurements (90 %) and the latest measurement (10 %).

Examples of the effect of filtering on output:

- Filtering factor 1.0 = No filtering, the latest measurement is output directly without integrating previous measurements.
- Filtering factor 0.5 = The reading output shows ~75 % of the measurement change after two two-second measurement cycles and ~93 % after four cycles.
- Filtering factor 0.1 = The reading output shows ~90 % of the measurement change after 22 measurement cycles.

The configuration range of the filtering factor is 0 ... 100 in the 16-bit register: for example, to set the factor to 0.5, set the value of the register to 50.

The following formula is used when calculating the output:

$$o_{\text{new}} = o_{\text{old}} + (m_{\text{new}} - o_{\text{old}}) \times f$$

o_{new}	New output
o_{old}	Previous output
m_{new}	New measurement
f	Filtering factor

Warranty

For standard warranty terms and conditions, see www.vaisala.com/warranty.

Please observe that any such warranty may not be valid in case of damage due to normal wear and tear, exceptional operating conditions, negligent handling or installation, or unauthorized modifications. Please see the applicable supply contract or Conditions of Sale for details of the warranty for each product.

Technical Support



Contact Vaisala technical support at helpdesk@vaisala.com. Provide at least the following supporting information:

- Product name, model, and serial number
- Name and location of the installation site
- Name and contact information of a technical person who can provide further information on the problem

For more information, see www.vaisala.com/support.

Recycling



Recycle all applicable material.



Follow the statutory regulations for disposing of the product and packaging.

VAISALA



Distributed by:

Kenelec Scientific Pty Ltd
1300 73 22 33
sales@kenelec.com.au
www.kenelec.com.au

www.vaisala.com

