
# CERTIFIER® FA VENTILATOR TEST SYSTEMS

FOR GAS FLOW ANALYSIS



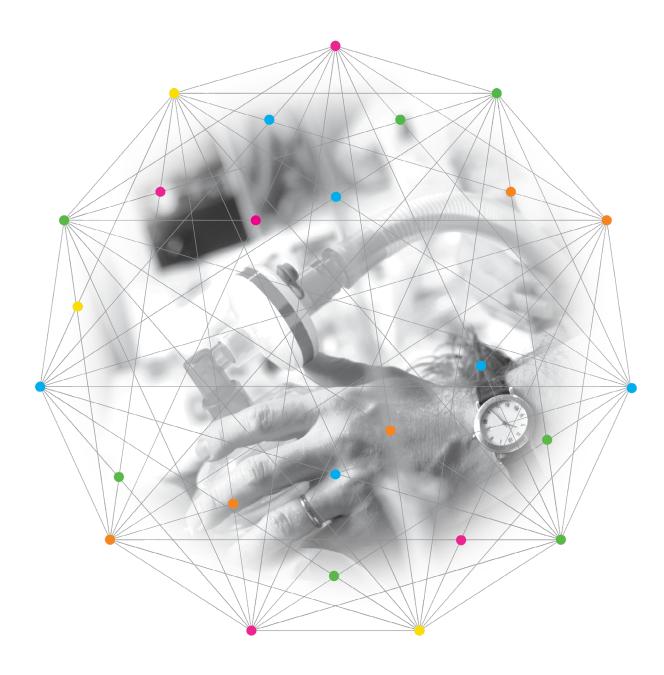

# IDEAL FOR HOSPITAL, HOME-CARE, FIELD SERVICE, LABORATORY AND MANUFACTURING

# CERTIFIER® FA PLUS VENTILATOR TEST SYSTEM

Certifier® FA Plus is the full-feature system capable of testing virtually all models of ventilators: adult, pediatric, anesthesia, neonatal and high-frequency.

# Highlights

- + Color touch screen graphical user interface
- + Real-time graphing mode
- + Bi-directional flow measurement
- + Data storage using SD Flash card and internal memory
- + Stored data accessible through USB interface
- + Report printing capability
- + Rechargeable battery plus


  AC operation

## **Test Parameters**


- + Flow
- + Peak & Minimum Flow
- + Volume (Inhaled and Exhaled)
- + Minute Volume
- + Low Pressure (Differential)
- + Peak & PEEP Pressure
- + Mean Airway Pressure
- + High Pressure
- + Barometric Pressure
- + Inspiratory Time
- + Expiratory Time
- + I:E Ratio
- + Respiratory Rate
- + Gas Temperature
- + Oxygen Concentration (with optional 4073 Kit)

Features	Certifier FA Plus
Gas Calibrations	Air, O <sub>2</sub> , Air/O <sub>2</sub> mixtures, N <sub>2</sub> , CO <sub>2</sub> , N <sub>2</sub> O
Flow Direction	Bi-Directional
Flow & Volume Modes	STP, ATP, BTPS, BTPD, plus user-defined
Temperature & Pressure Compensated	Yes
Max Breath Rate	1500 BPM
High Frequency Ventilators	Yes
High Pressure	-10 to 150 PSI (7 to 10 bar) Gauge
Low Pressure	-25 to 150 cm H <sub>2</sub> 0 Differential
Barometric Pressure	7 to 25 PSIA (500 to 1700 mbar)
Display	Color-Graphic Touch Screen
Batteries	Li-Ion Rechargeable Battery Pack
AC Adapter	Yes
Internal Memory	1 MB
SD Flash Card	Included
Computer Interface	USB
Printing	USB





Displays up to 18 test parameters



Graph up to 2 test parameters

# CERTIFIER FA VENTILATOR TEST SYSTEM

Certifier FA is a low-cost test system capable of testing multiple parameters of ventilator performance.

# Highlights

- + Simple, easy to read, user interface
- + Backlit LCD display
- + Entire kit weighs less than 3 lbs (1.4 Kg)
- + Volumes and flow in BTPS, ATP, or STP

# **Test Parameters**

- + Flow
- + Peak Flow
- + Volume
- + Stacked Volume
- + Minute Volume
- + Low Pressure
- + Peak & PEEP Pressure
- + Barometric Pressure
- + Inspiratory Time
- + I:E Ratio
- + Respiratory Rate
- + Oxygen Concentration (with optional 4073 Kit)

Features	Certifier FA
Gas Calibrations	Air, O <sub>2</sub> , Air/O <sub>2</sub> mixtures, N <sub>2</sub> O
Flow Direction	Uni-Directional
Flow & Volume Modes	STP, ATP, BTPS
Temperature & Pressure Compensated	Yes
Max Breath Rate	120 BPM
High Frequency Ventilators	_
High Pressure	_
Low Pressure	-25 to 150 cm H <sub>2</sub> 0 Gauge
Barometric Pressure	7 to 30 PSIA (500 to 2000 mbar)
Display	Fixed Segment LCD
Batteries	4-AA Alkaline Batteries
AC Adapter	_
Internal Memory	_
SD Flash Card	_
Computer Interface	_
Printing	-







4070 High-flow test system with 4073 Oxygen sensor kit (sold separately)

4080 High-flow test system with 4082 Low-flow kit (sold separately)

Certifier FA Plus		4062 LOW-110W KIT (SOID SEPARATELY)		
	Gas/Mode	Range	Accuracy**	
Flow-High Flow	Air, O <sub>2</sub>	-200 to +300 slpm*	±2% or ±0.075 slpm	
	Air/O <sub>2</sub> Mixtures	0 to 300 slpm	±4% or ±0.1 slpm	
	$N_2$	-200 to +300 slpm	±3% or ±0.1 slpm	
	CO <sub>2</sub>	-40 to +40 slpm	±3% or ±0.1 slpm	
Flow-Low Flow	Air, O <sub>2</sub>	0.01 to 20 slpm	±2% or ±0.01 slpm	
	N <sub>2</sub> , CO <sub>2</sub>	0.01 to 20 slpm	±3% or ±0.01 slpm	
	N <sub>2</sub> O	0.01 to 20 slpm	±4% or ±0.025 slpm	
Volume-High Flow-Inhaled	Air, O <sub>2</sub>	0.01 to 10 liters STP	±2% Plus 0.02 liters	
	Air/O <sub>2</sub> Mixtures	0.01 to 10 liters STP	±4% Plus 0.02 liters	
Volume-High Flow-Exhaled	Air, O <sub>2</sub>	0.01 to 10 liters STP	±3% Plus 0.03 liters	
	Air/O <sub>2</sub> Mixtures	0.01 to 10 liters STP	±4% Plus 0.04 liters	
Volume-Low Flow-Inhaled	Air, O <sub>2</sub>	0.01 to 10 liters STP	±2% or ±0.01 liters	
	$N_2O$	0.01 to 10 liters STP	±4% or ±0.01 liters	
Minute Volume- High Flow	-	0.01 to 100 liters STP	±3%	
Minute Volume- Low Flow	-	0 to 10 liters STP	±3%	
Respiratory Times	Ti, Tip, Te	0.04 to 30 seconds	±2% or ±0.01 seconds	
I:E Ratios	I:E, I:Eip	1:100 to 100:1	±4%	
Respiratory Rate	f	1 to 1500 breaths per minute	±2% or 0.1 bpm	
Low Pressure	All	-25 to +150 cm H <sub>2</sub> 0	±0.5% or ±0.15 cm H <sub>2</sub> 0	
High Pressure	_	-10 to +150 PSI (-0.7 to 10 bar)	±1% or 0.1 PSI (7 mbar)	
Barometric Pressure	_	7 to 23 PSI (500 to 1600 mbar)	±0.16 PSI (11 mbar)	
Oxygen Concentration	_	21% to 100%	2% of concentration	

TSI and the TSI Logo are registered trademarks of TSI Incorporated.

# Certifier FA

	Gas	Range	Accuracy**
Flow-High Flow Module	Air, O <sub>2</sub>	0 to 300 slpm*	±2% or ±0.075 slpm
	Air/O <sub>2</sub> Mixtures	0 to 300 slpm	±4% or ±0.1 slpm
Flow-Low Flow Module	Air, O <sub>2</sub>	0.01 to 15 slpm	±2% or ±0.01 slpm
	N <sub>2</sub> O	0.01 to 15 slpm	±4% or ±0.025 slpm
Volume-High Flow-Inhaled	Air, O <sub>2</sub>	0.01 to 10 liters STP	±2% Plus 0.02 liters
	Air/O <sub>2</sub> Mixtures	0.01 to 10 liters STP	±4% Plus 0.02 liters
Volume-Low Flow-Inhaled	Air, O <sub>2</sub>	0.01 to 9.999 liters STP	±2% or ±0.01 liters
	N <sub>2</sub> O	0.01 to 10 liters STP	±4% or ±0.01 liters
Minute Volume- High Flow	-	0.01 to 99 liters STP	±7%
Minute Volume- Low Flow	-	0 to 9.999 liters STP	±7%
Inspiratory Time	-	0.25 to 60 seconds	±0.01 seconds
I:E Ratio- High Flow	-	1:100 to 100:1	±5%
I:E Ratio- Low Flow	-	1:15 to 15:1	±5%
Respiratory Rate	-	0.5 to 120 breaths per minute	±5%
Low Pressure	_	-25 to +150 cm H <sub>2</sub> 0	±0.75% or ±0.2 cm H <sub>2</sub> 0
Barometric Pressure	-	7 to 29 PSI (500 to 2000 mbar)	±0.16 PSI (11 mbar)
0	I		

21% to 100%

2% of concentration

TO ORDER – CERTIFIER FA PLUS Model Description

Model

Oxygen Concentration

High-Flow Standard Kit 4080

**Optional Modules and Accessories** 

Model Description 4073 4082 Oxygen Sensor Kit Low-Flow Module

Part #

**Description** Extra battery pack and charger kit 1208061

1303860 Printer cable

TO ORDER - CERTIFIER FA

Model

Description High-Flow Standard Kit 4070

Optional Modules and Accessories
Model Description
4073 Oxygen Sensor Kit 4072 Low-Flow Module

Part # Description

1319288 Hard shell carrying case



**TSI Incorporated** - Visit our website **www.tsi.com** for more information.

Tel: +1 800 874 2811 **Tel:** +91 80 67877200 USA India Tel: +44 149 4 459200 **Tel:** +86 10 8251 6588 UK China Tel: +33 4 91 11 87 64 France **Singapore Tel:** +65 6595 6388

Germany Tel: +49 241 523030 measuring up

Printed in U.S.A.

Distributed by:

Kenelec Scientific Pty Ltd 1300 73 22 33 sales@kenelec.com.au www.kenelec.com.au

<sup>\*</sup> slpm = Standard Liters per Minute
\*\*Accuracy stated as a percent of reading at TSI standard gas conditions. See operators manual for more complete specifications