



® Knowledge
Beyond
Measure.

Versatile Water-Based Condensation Particle Counter


Model 3789



Reliable Under (Under) Pressure

We tested this new Water-Based Condensation Particle Counter (WCPC) to the extreme and can confidently say that this one is more robust than ever.

Our reliability testing consisted of operating a valve at the CPC's inlet to close the inlet completely for 10 seconds, every 5 minutes, for 5 days. This created large pressure drops which would cause problems for many other instruments. The new Versatile Water-based CPC recovered every single time, accurately measuring the particle number concentration as if nothing had happened.

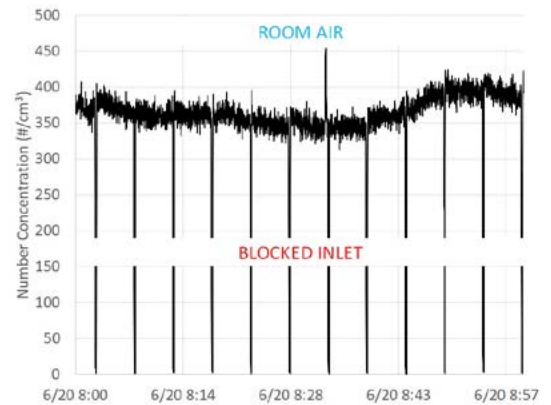

Lower Maintenance

With the new wick and water handling design, the operation time is now six months with the same wick. While the new design can even stand up to tap water, we still recommend using distilled water to reach and exceed the six-month lifetime.



Successfully passed pressure test (see "Reliable Under (Under) Pressure" above)

How it Works

4. Counting

The enlarged particles pass through a laser beam and scatter light. Each pulse of scattered light is counted individually.

3. Moderation


Even after the condensation step in #2, some vapor-phase water remains. The moderator stage condenses this water out of the vapor phase and onto the walls of the wick. This allows that water to be re-used, and also protects the optics (#4) from condensation.

2. Growth

The sample moves through a humid chamber where it becomes supersaturated, forcing water vapor to condense onto the cooled particles. The particles are now large enough to be detected when they pass through the laser beams in #4.


1. Conditioning

The aerosol moves through a humid chamber to surround the particles with water vapor.

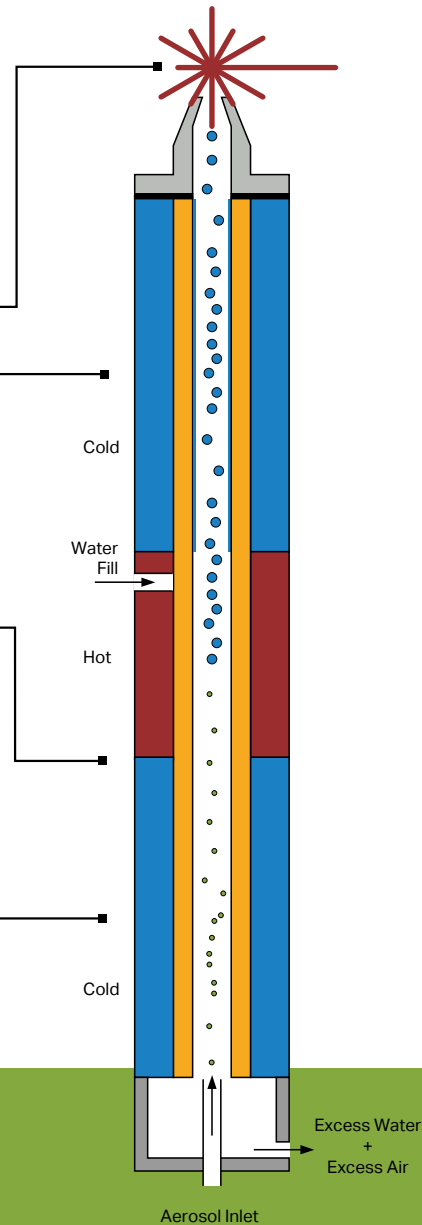

Reliable At High Concentration

Another test was challenging the WCPC with aerosol concentrations close to its maximum concentration range for 10 consecutive days. Every 15 minutes a reference butanol-based CPC was used to check the accuracy of the particle concentration reading. Despite being continuously challenged with a high aerosol concentration, the new water-based CPC provided stable measurements throughout the test.

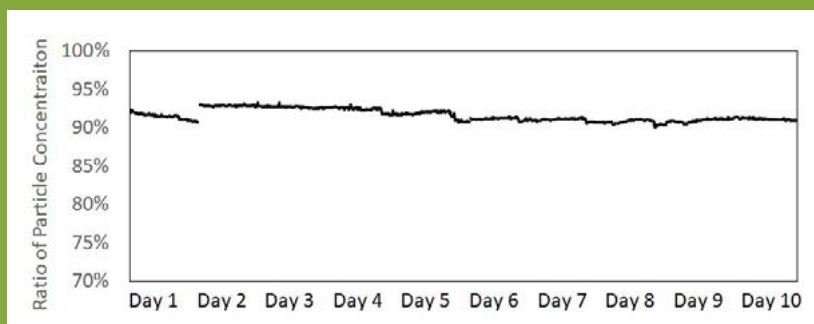

Selectable Particle Size Cut-Off

No more deciding between fixed counting efficiencies. The new Versatile Water-based CPC provides selectable particle size-cut-off options: 2 nm and 7 nm for D50%. Furthermore, a custom setting can be stored. For particle detection near 1 nm see publication: Hering et al. (2017) Aerosol Science and Technology, 51:3, 354-362.

Features and Specifications

Selectable Particle Size Cut-Off (D50%)

2.2 nm, 7 nm, custom

Particle Concentration Range

Up to 200,000 particles/cm³

Particle Concentration Accuracy

±5% at <200,000 particles/cm³

Inlet flow

0.6, 1.5, or 2.5 L/min (option)

Aerosol flow


0.3 L/min

Data rate

50 Hz

Internal memory for up to 1 year.
Remote control via Ethernet option.

TSI and the TSI logo are registered trademarks of TSI Incorporated in the United States and may be protected under other country's trademark registrations.

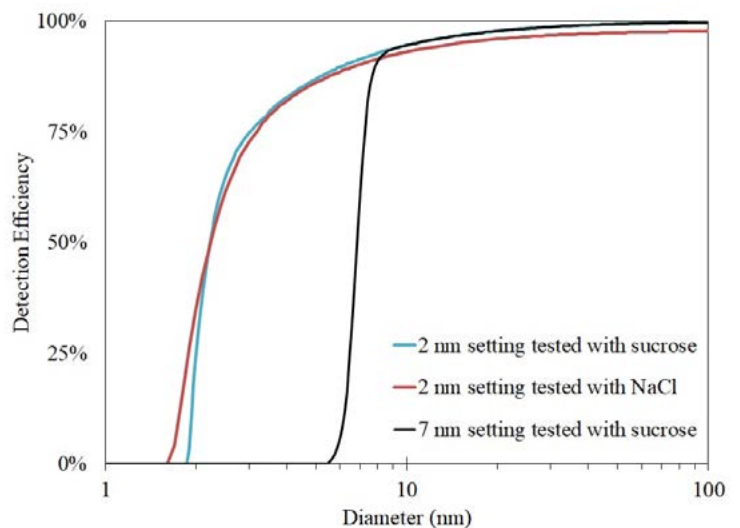

Learn more at tsi.com/wcpc



Knowledge Beyond Measure.

TSI Incorporated - Visit our website www.tsi.com for more information.

USA Tel: +1 800 874 2811
UK Tel: +44 149 4 459200
France Tel: +33 1 41 19 21 99
Germany Tel: +49 241 523030

India Tel: +91 80 67877200
China Tel: +86 10 8219 7688
Singapore Tel: +65 6595 6388



Distributed by:

Kenelec Scientific Pty Ltd
1300 73 22 33
sales@kenelec.com.au
www.kenelec.com.au